

# **NREL Pyrheliometer Comparisons September 23 – October 4, 2002**

**(NPC-2002)**

## **Final Report**

By

Ibrahim Reda  
Tom Stoffel  
Steve Wilcox

National Renewable Energy Laboratory  
Electric & Hydrogen Technologies & Systems Center  
Resource Integration Group  
Measurement & Instrumentation Team



September 17, 2003

## **NOTICE**

This report was prepared as an account of work sponsored by an agency of the United States government. Neither the United States government nor any agency thereof, nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States government or any agency thereof. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States government or any agency thereof.

## NPC 2002 Participants



Tom Stoffel, Wim Zaaiman, Duncan Maciver, Craig Webb, Bob Heiskell, Jim Goza, Fred Denn, Jim Treadwell, Ibrahim Reda [Not pictured: Gary Hodges, Joe Michalsky, Bill Miller]

## Acknowledgements


We sincerely appreciate the support of Susan Hock, our Center Director, for helping us host these comparisons. Our thanks go to Beverly Kay for her timely administrative and logistical help, Pete Gotseff for his site and instrument preparations, and to Afshin Andreas for providing web-access to Baseline Measurement System data. We are also grateful to Stan Bull and Daryl Myers for their financial support from NREL's Metrology Laboratory Technical Overhead and the DOE/NREL Photovoltaics Research Program. The DOE Atmospheric Radiation Measurement (ARM) Program, funded through Argonne National Laboratory and Pacific Northwest National Laboratory, provided additional support. Solar irradiance measurements from radiometers with direct traceability to the World Radiometric Reference (WRR) were provided by Wim Zaaiman (European Solar Testing Installation), Don Nelson (NOAA's Climate Monitoring & Diagnostics Laboratory), Chris Cornwall and Gary Hodges (NOAA's Surface Radiation Research Branch), Jerry Maybee and Gene Zerlaut (ATLAS/DSET), and Joe Michalsky (SUNYA/ASRC). These radiometers greatly strengthened our ability to transfer the WRR to the participating radiometers. Our thanks also go to each participant for their patience and cooperation during this weather-dependent exercise.

This work was accomplished under NREL subtasks PV27401, WU1D5600, WU865600, and 20100010.

# NREL Solar Radiation Research Laboratory (SRRL)



Northwest View

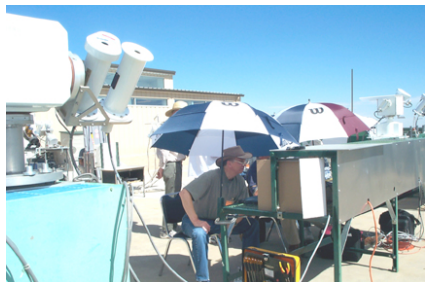

Joe Michalsky



Wim Zaaiman




Fred Denn



Jim Goza



Jim Treadwell

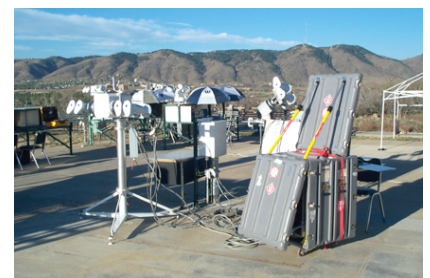

Transfer Standard Group

## Table of Contents

Acknowledgements .....	iii
Abstract .....	vi
1. Introduction .....	1
2. Reference Instruments .....	2
3. Measurement Protocol .....	2
4. Transferring World Radiometric Reference .....	3
4.1 Calibration Requirements .....	3
4.2 Determining the Reference Irradiance .....	3
4.3 Data Analysis Criteria .....	4
4.4 Measurements .....	4
4.5 Results .....	4
4.6 Recommendations .....	17
5. Ancillary Data .....	17
6. References .....	18
7. Images .....	18
8. Appendices	
A. List of Participants and Pyrheliometers .....	A-1
B. Ancillary Data Summaries .....	B-1
23 September 2002 .....	B-1
24 September 2002 .....	B-2
25 September 2002 .....	B-3
26 September 2002 .....	B-4
C. Operational Notes .....	C-1

## Abstract

Providing reliable measurements of solar irradiance places many demands on the operator of commercially available radiometers. Maintaining accurate radiometer calibrations traceable to an international standard is the first step in producing research-quality solar irradiance measurements.

In 1977, the World Meteorological Organization (WMO) established the World Radiometric Reference (WRR) as the international standard for solar irradiance measurement. The WRR is a detector-based measurement standard, subject to instrument performance changes with time. Therefore, every five years, the World Radiation Center/Physikalisch-Meteorologisches Observatorium Davos (WRC/PMOD) in Davos, Switzerland hosts an International Pyrheliometer Comparison (IPC) for transferring the WRR to participating radiometers. Representing the U.S. Department of Energy, NREL has participated in each of the IPCs since 1980. As a result, NREL has developed and maintained a select group of absolute cavity radiometers with direct calibration traceability to the WRR. These instruments are then used to transfer WRR to other radiometers.

NREL Pyrheliometer Comparisons (NPCs) are held annually at the Solar Radiation Research Laboratory (SRRL) in Golden, Colorado. Open to any pyrheliometer owner/operator, the NPC provides an opportunity to determine the unique WRR Transfer Factor (WRR-TF) for each participating pyrheliometer. By adjusting all subsequent solar irradiance measurements by the appropriate WRR-TF, the operator can establish calibration traceability to the WRR.

NPC-2002 was scheduled at from September 23 through October 4, 2002. Twelve participants operated 23 absolute cavity radiometers and two conventional thermopile-based pyrheliometers to simultaneously measure clear-sky direct normal solar irradiance during this period. The Transfer Standard Group (TSG) of reference radiometers for NPC-2002 consisted of five radiometers with direct traceability to the WRR because each unit had participated in IPC-IX 2000. As the result of NPC-2002, each participating absolute cavity radiometer was assigned a new WRR-TF computed as the ratio of observed irradiance to the corresponding reference irradiance as determined by the TSG. The performance of the TSG during NPC-2001 was consistent with previous comparisons, including the latest IPC-IX. The measurement performance of the TSG allowed the transfer of the WRR to each participating radiometer with an estimated uncertainty of  $\pm 0.32\%$  with respect to SI units.

The comparison protocol is based on data collection periods, or “runs.” Each run consists of a six-minute electrical self-calibration, a series of 33 solar irradiance measurements at 20-second intervals, and a post-calibration. More than 800 reference irradiance measurements for each participating radiometer were collected during NPC-2002. Clear-sky direct normal irradiance levels ranged from less than  $700 \text{ Wm}^{-2}$  to  $980 \text{ Wm}^{-2}$ .

Ancillary environmental parameters (e.g., broadband irradiance, spectral irradiance and other surface meteorological data) collected at SRRL during the comparison are also presented in this report to document the environmental test conditions.

Future comparisons are planned annually at SRRL to ensure worldwide homogeneity of solar radiation measurements traceable to the WRR.

## 1. Introduction

Collecting solar irradiance data for applications in renewable energy technology research, global climate change studies, satellite remote sensing validations, general atmospheric science research, or the myriad of other possibilities, requires measurements traceable to a recognized calibration standard. The World Radiometric Reference (WRR) is the internationally recognized standard for solar irradiance measurements [Fröhlich, 1991].

The WRR was established by the World Meteorological Organization (WMO) in 1977 and has been maintained by the World Radiation Center at the Physikalisch-Meteorologisches Observatorium Davos (WRC/PMOD) in Switzerland (<http://www.pmodwrc.ch>). This standard of measurement is maintained for broadband solar irradiance with an absolute uncertainty of better than  $\pm 0.3\%$  with respect to the System International (SI) unit [Romero, et al, 1996]. This standard is widely used for the calibration of shortwave radiometers (pyranometers and pyrhemometers) with a wavelength response range of 280 nm to 3000 nm. Every five years, the WRR is transferred to WMO Regional Centers and other participants in the International Pyrhemometer Comparisons (IPC) held at the WRC/PMOD. The instantaneous measurements from the seven radiometers comprising the World Standard Group (WSG) are compared at 90-second intervals with the data from participating radiometers recorded under clear-sky conditions. Maintaining the mean WRR of the seven WSG radiometers, a WRR Transfer Factor is calculated for each of the participating radiometers [Reda, 1996]. The range of historical WRR Transfer Factors is  $1.00000 \pm 0.00250$ . Multiplying the irradiance reading of each radiometer by its assigned WRR Transfer Factor (WRR-TF) will result in measurements that are traceable to WRR and therefore consistent with the international reference of solar radiation measurement.

The 2002 NREL Pyrhemometer Comparisons (NPC-2002) were scheduled from September 23 to October 3, 2002 at the Solar Radiation Research Laboratory (SRRL) in Golden, Colorado. Twelve participants operated 23 absolute cavity radiometers during the comparisons (see Appendix A for list of participants). The following organizations were represented at NPC-2002:

- Analytical Services and Materials, Inc.
- Atlas Weathering Services, Inc. -DSET Laboratories
- Atmospheric Radiation Measurement Program of the U.S. Department of Energy
- European Commission Directorate General JRC
- Lockheed Martin Technical Operations
- NASA Langley Research Center, Atmospheric Sciences Division
- National Oceanic and Atmospheric Administration
  - Climate Monitoring & Diagnostics Laboratory
  - Surface Radiation Research Branch
- National Renewable Energy Laboratory
  - Electric & Hydrogen Technologies & Systems Center
  - Metrology Laboratory
  - Photovoltaic Research Program
- State University of New York at Albany, Atmospheric Sciences Research Center

Weather conditions during the period September 23-25 were adequate for this year's NPC (see Appendix B for more specific meteorological information). The results presented in this report are based on clear-sky direct normal solar irradiance data collected on these three days.

## 2. Reference Instruments

Five absolute cavity radiometers that participated in IPC-IX were used as the Transfer Standard Group (TSG) to maintain the WRR for this comparison. Although additional radiometers with IPC-IX history were available, only those instruments within NREL's control were selected for the TSG. This will permit long-term continuity of the TSG while providing adequate statistical representation of the WRR. NPC results from other radiometers with direct traceability to an IPC provide assurance to our process for establishing the WRR. Table 2.1 is a list of the TSG absolute cavity radiometers with their *WRR Transfer Factors* and *Pooled Standard Deviations* as determined from the latest International Pyrheliometer Comparisons in 2000 [WRC/PMOD, 2001].

**Table 2.1 IPC-IX Results Summary for the NPC-2002 TSG**

Serial Number	WRR Factor (from IPC-IX)	Standard Deviation (%)	Number of Readings
AHF 28553	0.99733	0.049	212
AHF 28968	0.99866	0.062	113
AHF 29220	0.99846	0.063	113
AHF 30713	0.99861	0.059	113
TMI 68018	0.99848	0.053	113
<b>Mean WRR for the TSG</b>	0.99831	<b>Pooled Std Deviation for the TSG 0.056%</b>	

The Pooled Standard Deviation ( $SD_p$ ) for the Transfer Standard Group (TSG) is computed from the following equation:

$$SD_p = \left[ \frac{\sum_{i=0}^m (n_i * S_i^2)}{\sum_{i=0}^m n_i} \right]^{1/2}$$

where,

- i =  $i^{\text{th}}$  cavity
- m = number of reference cavities
- $S_i$  = standard deviation of the  $i^{\text{th}}$  cavity, from IPC-IX
- $n_i$  = number of readings of the  $i^{\text{th}}$  cavity, from IPC-IX

## 3. Measurement Protocol

The decision to deploy instruments for a comparison is made daily. Data are collected only during clear-sky conditions determined visually and from stability of pyrheliometer readings. Simultaneous direct normal solar irradiance measurements were taken by most cavity radiometers in groups of 33 observations at 20-second intervals (PMO6 used 40-second open/closed shutter cycle). Each group of observations is called a *Run*. An electrical self-calibration of each absolute cavity is performed just prior to each Run. Previous WRR-TFs were not applied to the observations. The original manufacturer calibration factor was used according to the standard operating procedure provided by the manufacturer for each radiometer. A timekeeper announced the beginning of calibration periods and gave a 6-minute countdown prior to the start of each Run to facilitate the simultaneous start for each participant (See Appendix C for details).



By consensus, the goal was set to acquire at least 300 observations from each radiometer to determine the WRR-TF. Participants also agreed that ten Runs should be made over a period of at least two days to provide a variety of temperature and spectral irradiance conditions. Our goal was to build a statistically significant data set from which to derive individual WRR TF.

Data from each radiometer/operator system are collected at the end of the day using diskettes. Daily summaries were produced using a spreadsheet analysis tool. Results were distributed to the participants the following day. Additional operational notes can be found in Appendix C.

#### **4. Transferring World Radiometric Reference**

The primary purpose of these absolute cavity comparisons is to transfer the WRR from the NPC Transfer Standard Group (TSG) to each of the participating radiometers. This requires the collection of simultaneous measurements of clear-sky direct normal (or beam) solar irradiance by the participating radiometers and the TSG.

##### 4.1 Calibration Requirements

Using WMO guidelines [Romero, 1995], the following conditions were required before data collection was accomplished during NPC-2002:

- Radiation source was the sun, with irradiance levels greater than 700 Wm<sup>-2</sup>
- Digital multimeters with accuracy better than 0.05% of reading were used to measure the thermopile signals from each radiometer
- Solar trackers were aligned within  $\pm 0.25^\circ$  slope angle
- Wind speed was low ( $< 5$  m/s) from the direction of the solar azimuth  $\pm 30^\circ$
- Cloud cover was less than 1/8 with an angular distance larger than  $15^\circ$  from the sun.

##### 4.2 Determining the Reference Irradiance

Five absolute cavity radiometers, that participated in IPC-IX, were used as the TSG to transfer the WRR in the comparison. The WRR Transfer Factor for each of the TSG is presented in Table 2.1. The reference irradiance at each reading is calculated using the following summarized steps [Reda, 1996]:

- a. Each irradiance reading of the TSG is divided by the irradiance measured by AHF28553, the instrument with the *lowest* standard deviation with respect to the WRR.
- b. Maintaining the mean of WRR for the TSG, a new WRR Transfer Factor for NPC-2002 is recalculated for each of the TSG cavities [Reda, 1996].
- c. The reference irradiance for each 20-second observation in a Run is computed as the mean of the simultaneous reference irradiances measured by the TSG. The reference irradiance reading for each cavity in the TSG is the irradiance reading of the cavity multiplied by its new WRR Transfer Factor calculated in step b.

### 4.3 Data Analysis Criteria

The absolute cavity radiometer AHF30713 was used to check irradiance stability at the time of each comparison reading. Stable irradiance readings are defined to be within  $1.0 \text{ Wm}^{-2}$  during an interval of three seconds centered about the comparison reading, i.e., one second before and one second after the recorded reading. Unstable irradiance readings are marked in the data record and automatically rejected from the data analysis. Historically, this has affected less than 10% of the data collected during an NPC.

Additionally, all calculated ratios of the reference irradiance divided by the test instrument irradiance that deviated from their mean by more than 1.0% were rejected [WRC/PMOD, 1996]. Typically, data rejected from the analysis in this manner were the result of failed tracker alignment, problems with the pre-calibration, or similar cause for a bias greater than expected from a properly functioning absolute cavity radiometer.

### 4.4 Measurements

NPC-2002 was scheduled for September 23 - October 4, 2002. The comparisons were completed on September 25<sup>th</sup> after more than 800 data points were collected from 24 runs completed during three days with the requisite clear-sky conditions. The actual number of readings for each participating radiometer compared with the reference irradiance varies according to the data analysis selection criteria described above. Additionally, some instruments experienced minor data loss due to a variety of problems with the measurement systems and operating difficulties.

### 4.5 Results

The results for the TSG are presented in Table 4.5.1. To evaluate the performance of these instruments, the standard deviations of each radiometer are monitored during the comparisons. The results suggest successful performance of the TSG during this NPC:

- The NPC2002 WRR Transfer Factors did not change by more than a fraction of the standard deviation derived during IPC-IX in 2000 (see Table 2.1 for IPC-IX results).
- The standard deviations of the new WRR Transfer Factors are also smaller than the standard deviations observed for these instruments during IPC-IX.

The WRR Transfer Factor for each participating cavity radiometer is derived using the reference irradiance values derived from the TSG. At each reading, the reference irradiance is divided by the irradiance measured by a participating radiometer. The mean of these ratios is the WRR Transfer Factor for each participating radiometer. Results for each radiometer participating in NPC2002 are presented in Table 4.5.2.

**Table 4.5.1 Summary Results for the Reference Transfer Standard Group (TSG) Radiometers Used for NPC2002**


Serial Number	WRR-IPCIX	WRR-NPC2002	St. Dev.	Number of Readings
AHF28968	0.99866	0.99870	0.00	837
AHF29220	0.99846	0.99868	0.03	837
AHF30713	0.99861	0.99850	0.04	837
TMI68018	0.99848	0.99833	0.08	837
Mean WRR	0.99855	0.99855		

**Table 4.5.2 Results for Radiometers Participating in NPC2002**

Serial Number	WRR-TF NPC2002	sd%	Number of Readings	U95%	
				w.r.t. WRR	w.r.t. SI
17142	0.99865	0.08	749	0.19	0.36
23734	0.99892	0.05	833	0.15	0.34
28552	0.99816	0.09	661	0.22	0.37
28553	0.99724	0.05	606	0.15	0.34
28964	0.99862	0.06	740	0.17	0.35
29222	1.00060	0.05	796	0.16	0.34
30495	0.99787	0.05	796	0.16	0.34
30710	1.00002	0.06	798	0.17	0.34
31041	0.99785	0.06	810	0.17	0.34
31104	1.00040	0.04	831	0.15	0.33
31105	1.00357	0.07	816	0.18	0.35
32452	0.99908	0.06	837	0.18	0.35
67502	1.00053	0.08	611	0.20	0.36
68017	1.00020	0.07	731	0.18	0.35
68020	0.99721	0.12	720	0.27	0.40
69036	1.00250	0.15	99	0.33	0.45
PMO6 81109	0.99938	0.07	220	0.19	0.36
PMO6 911204	1.00034	0.09	221	0.21	0.37

Note: No results are available for AWX 32448.

## WRR for NREL Reference Cavities

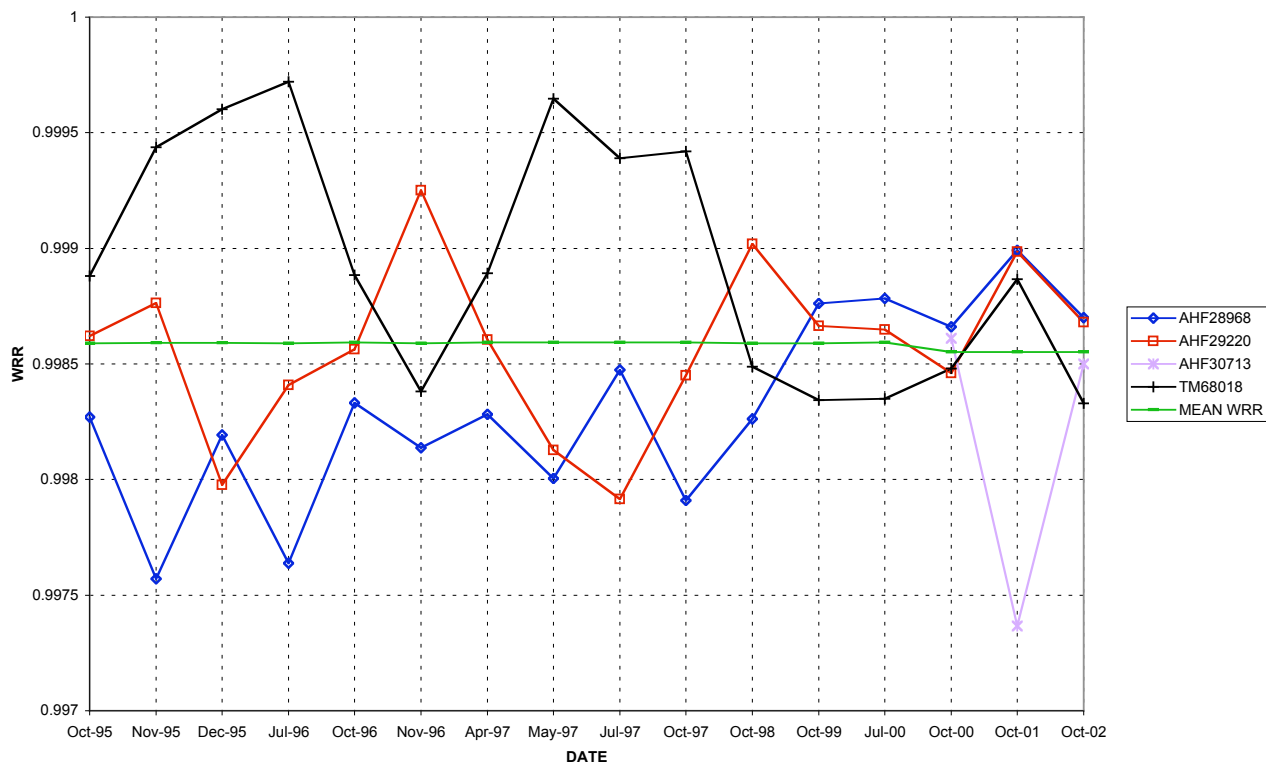

The uncertainty of the WRR Transfer Factors associated with each participating radiometer with respect to the WRR is calculated using the following formula:

$$U_{95} = \pm [(2 * 0.104)^2 + (2 * SD)^2]^{1/2}$$

where,

- $U_{95}$  = Uncertainty of the WRR Transfer Factor (in percent) determined at NPC2002 with 95% confidence level
- 0.104 = Pooled standard deviation of the six reference radiometers that participated in IPC-IX (September/October 2000).
- SD = One standard deviation of the WRR Transfer Factor (in percent) determined at NPC2001 for each participating cavity.


The uncertainty of the WRR Transfer Factors associated with each participating radiometer with respect to SI units was calculated using the following formula:



$$U_{95} = \pm [(0.3)^2 + (2 * 0.104)^2 + (2 * SD)^2]^{1/2}$$



where,



- 0.3 is the uncertainty ( $\pm\%$ ) of the WRR scale with respect to SI units.

The statistical analyses of WRR Transfer Factors for 18 participating radiometers are presented in Figures 4.5.1 through 4.5.18. These graphical summaries indicate the mean, standard deviation, and frequency of occurrence of the WRR Transfer Factors determined during NPC2002.


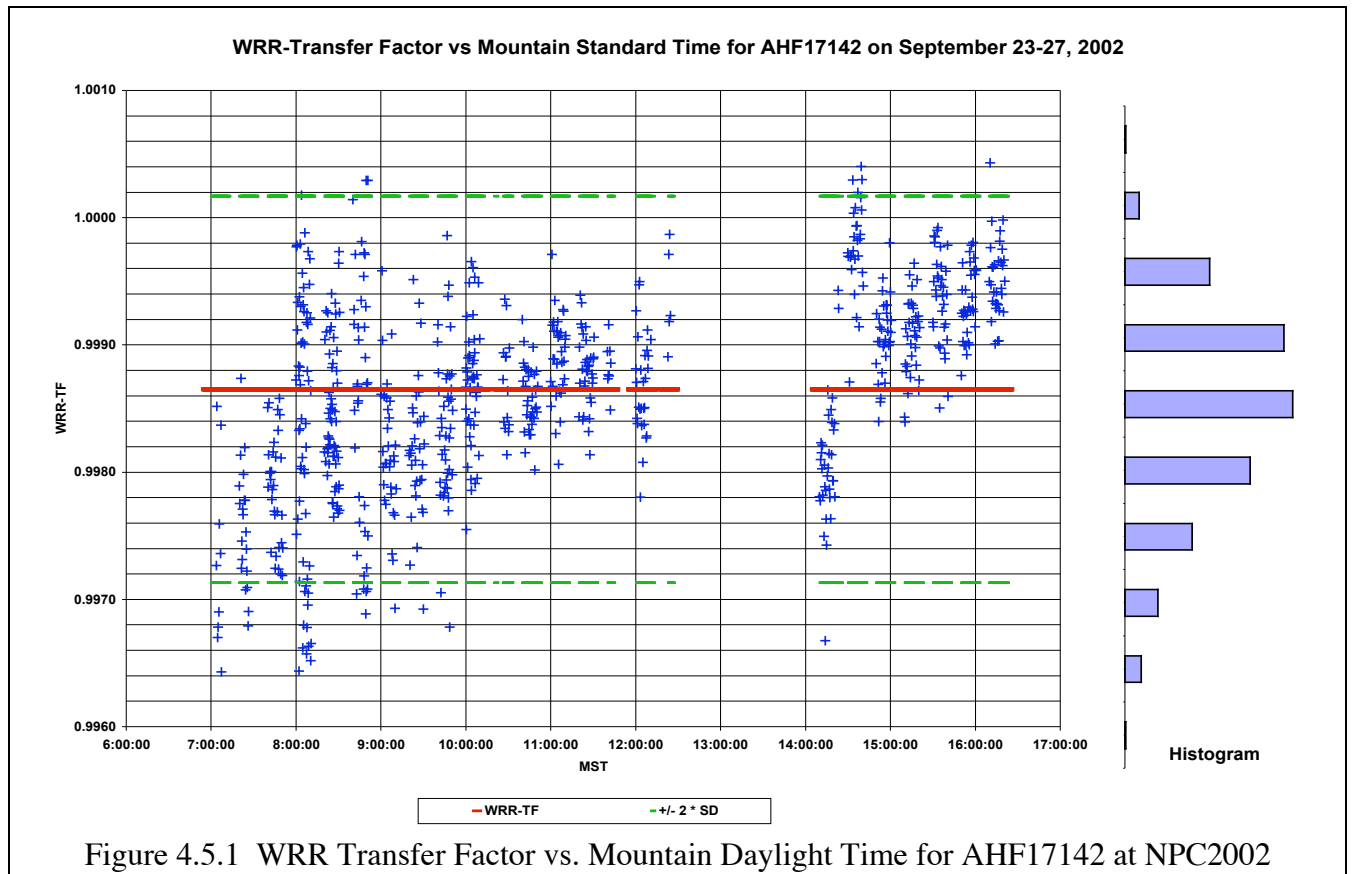


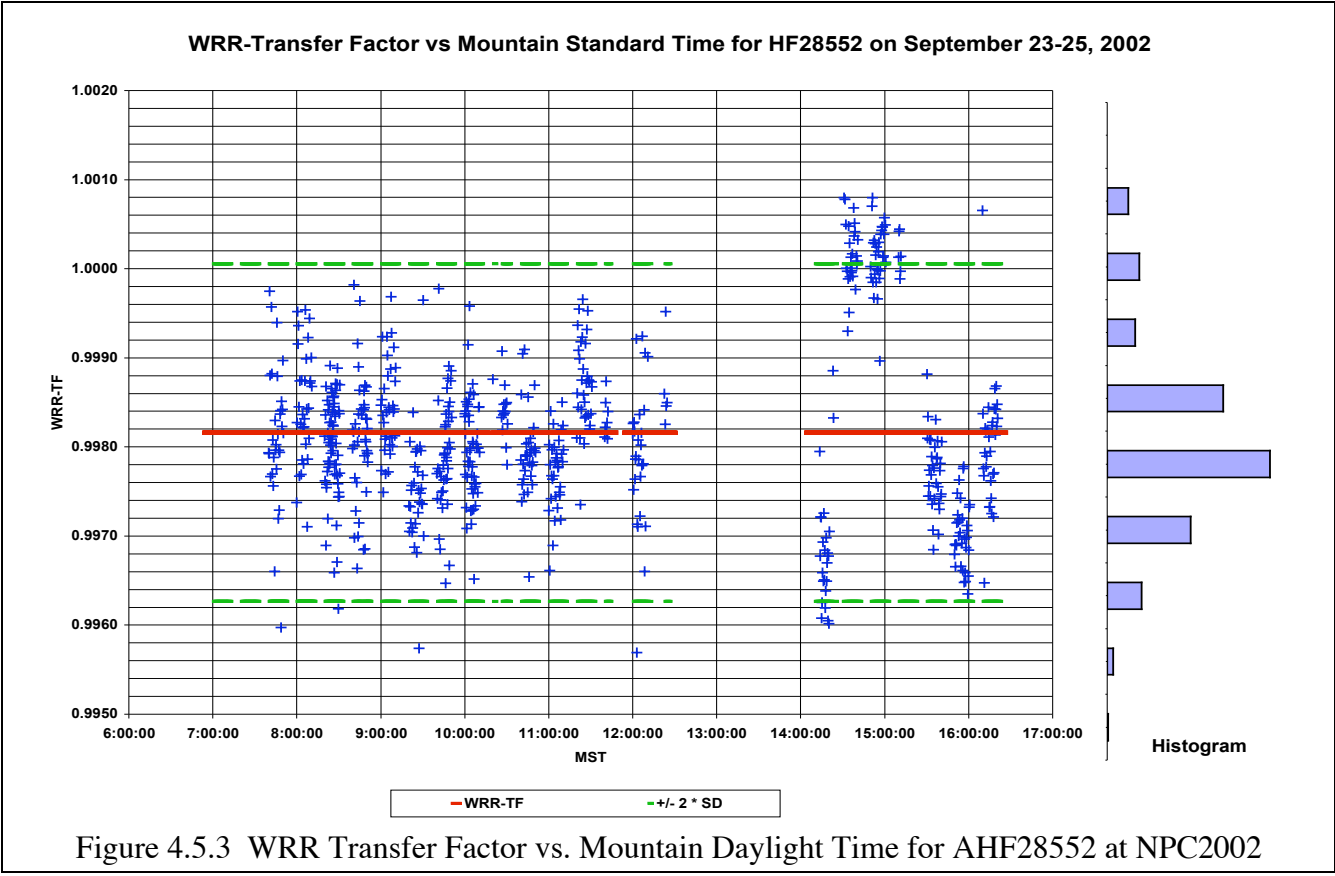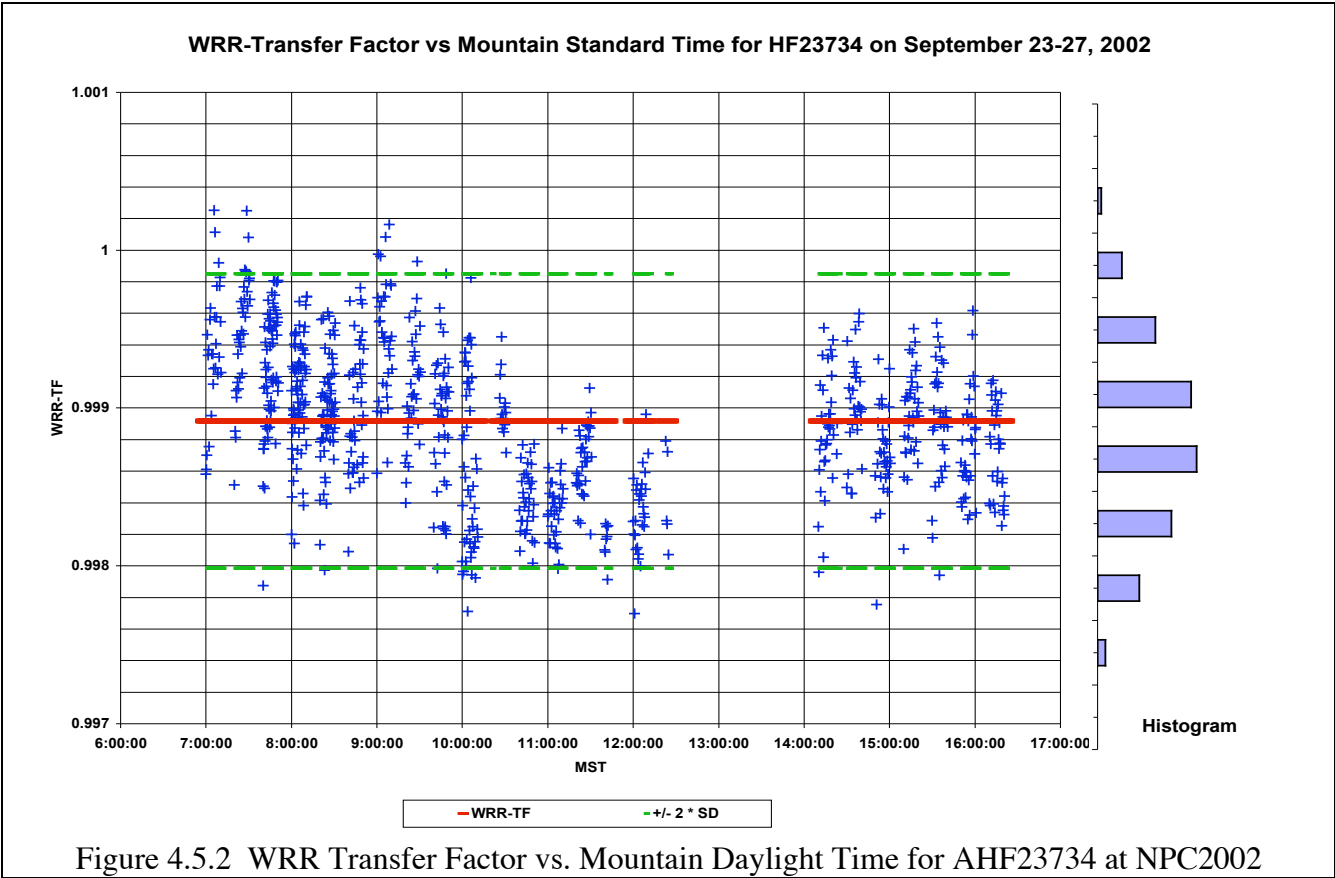

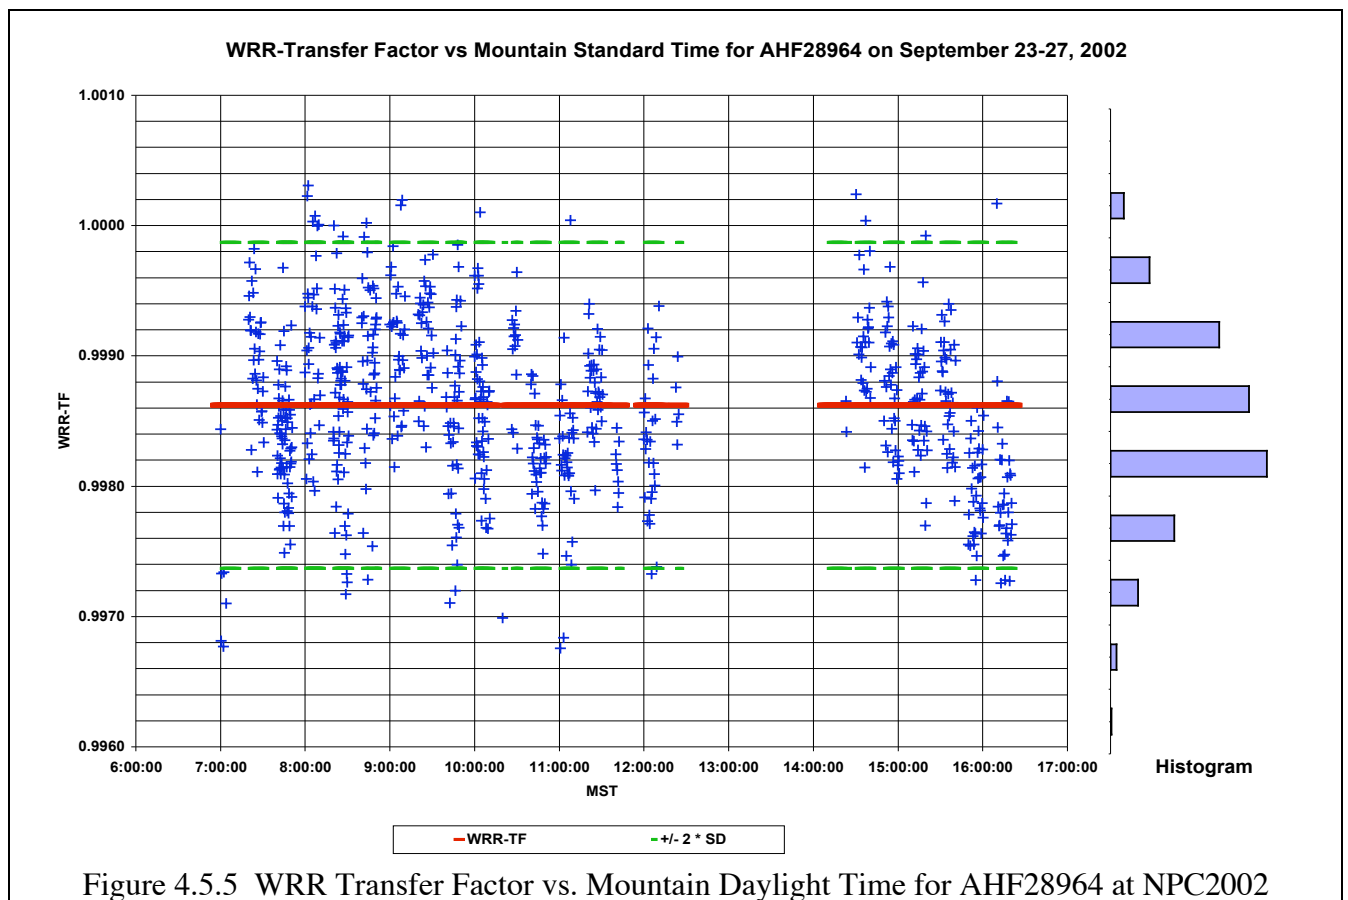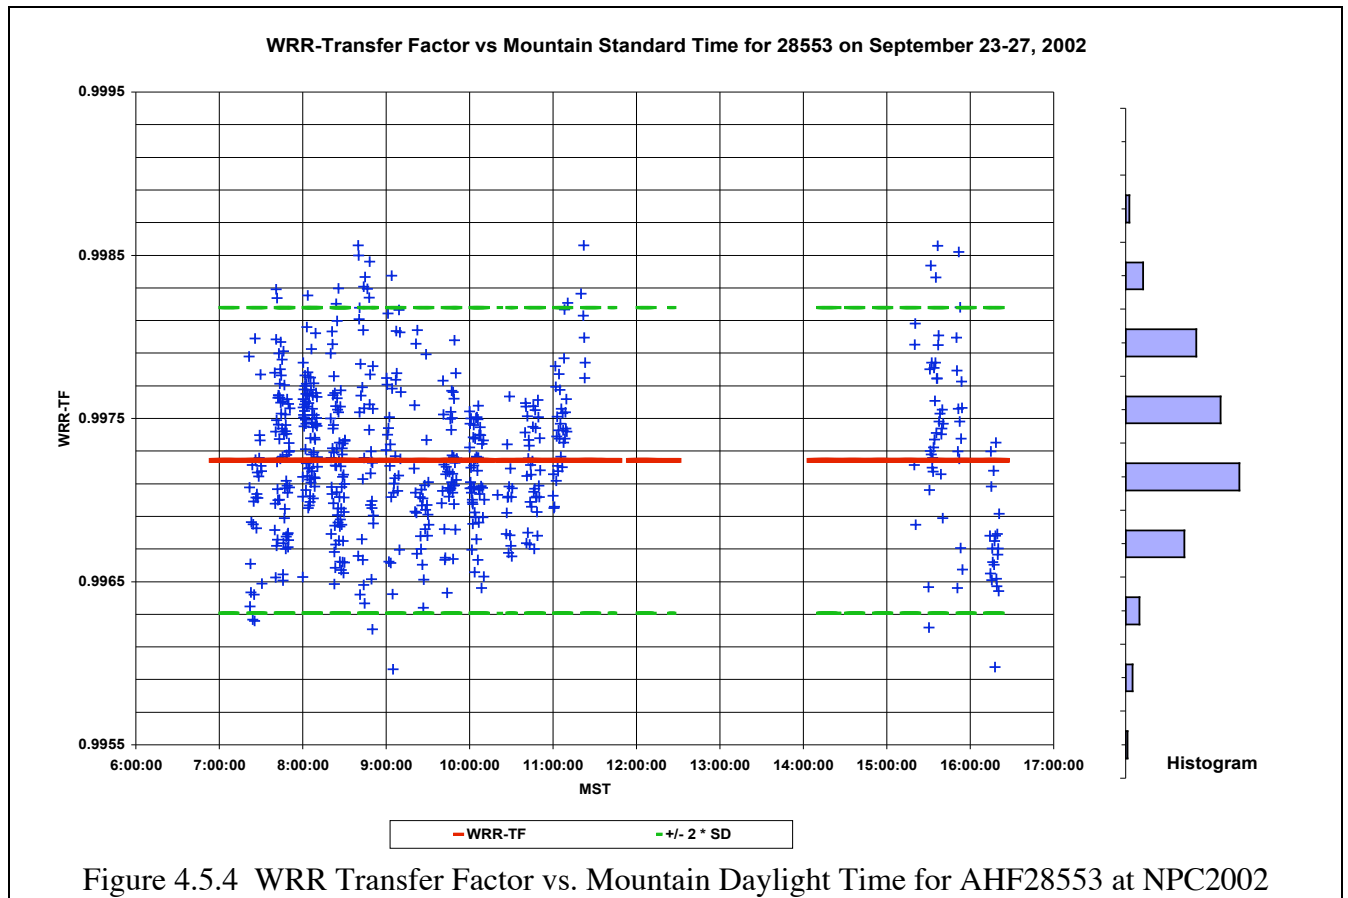

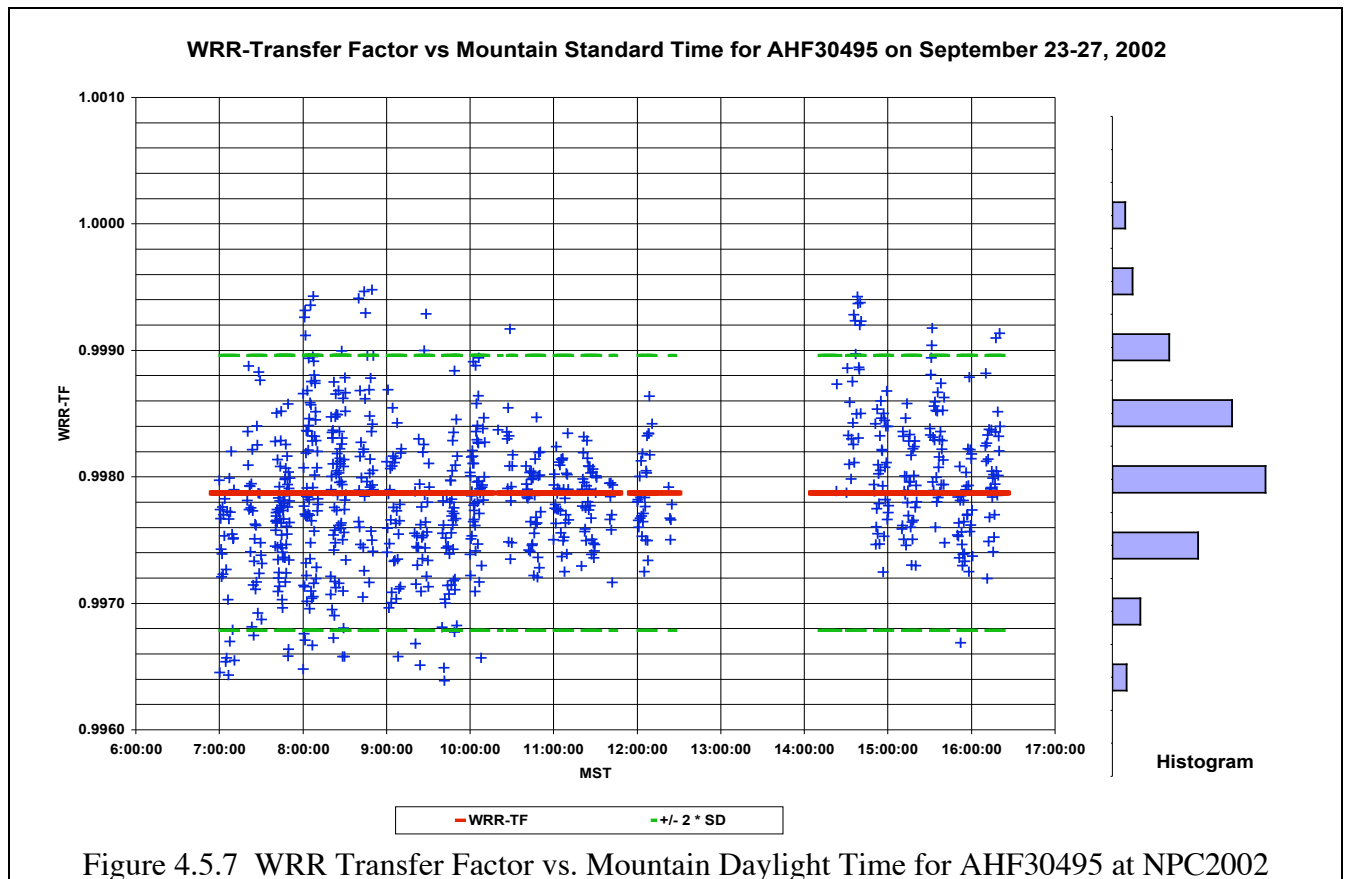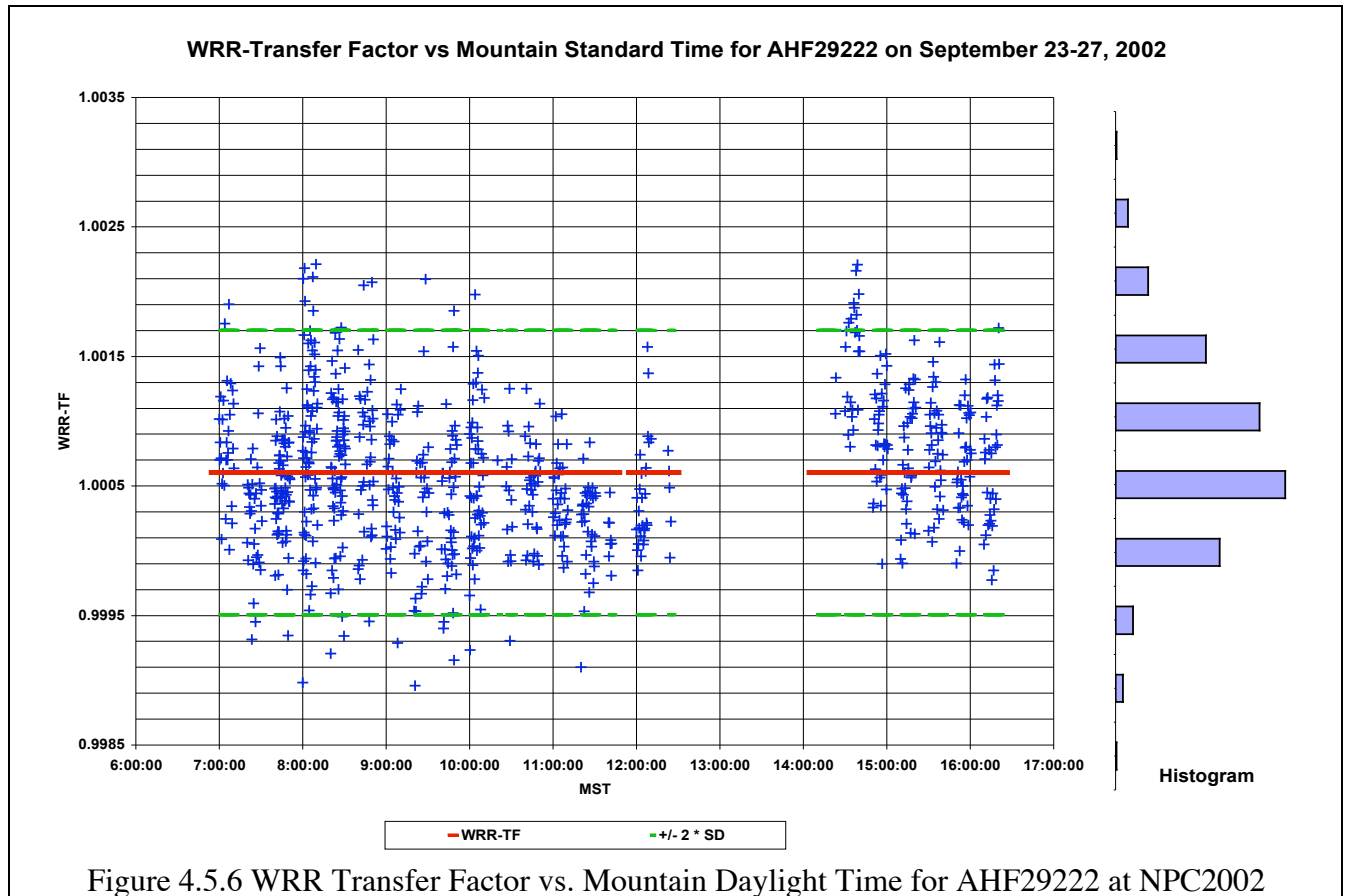



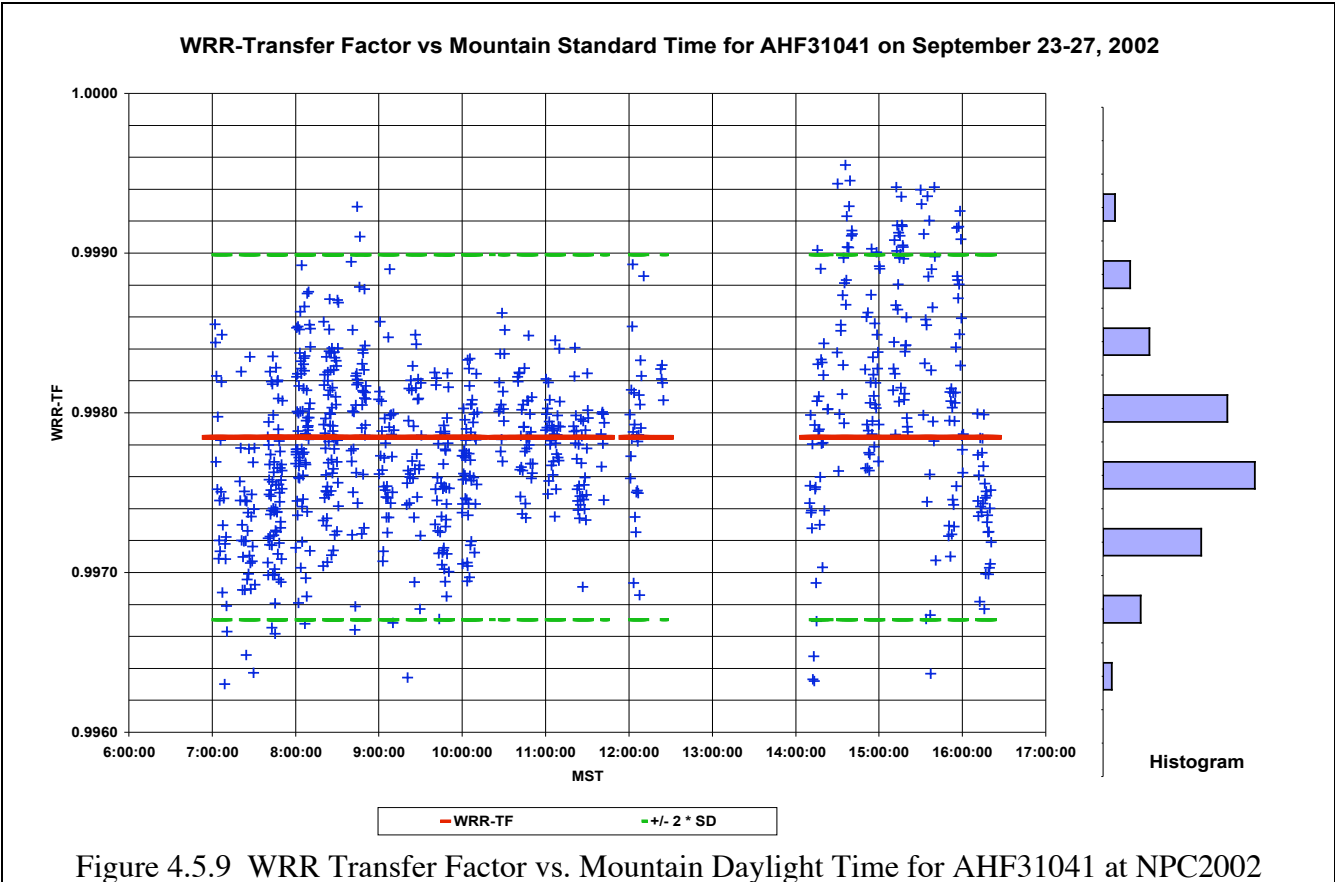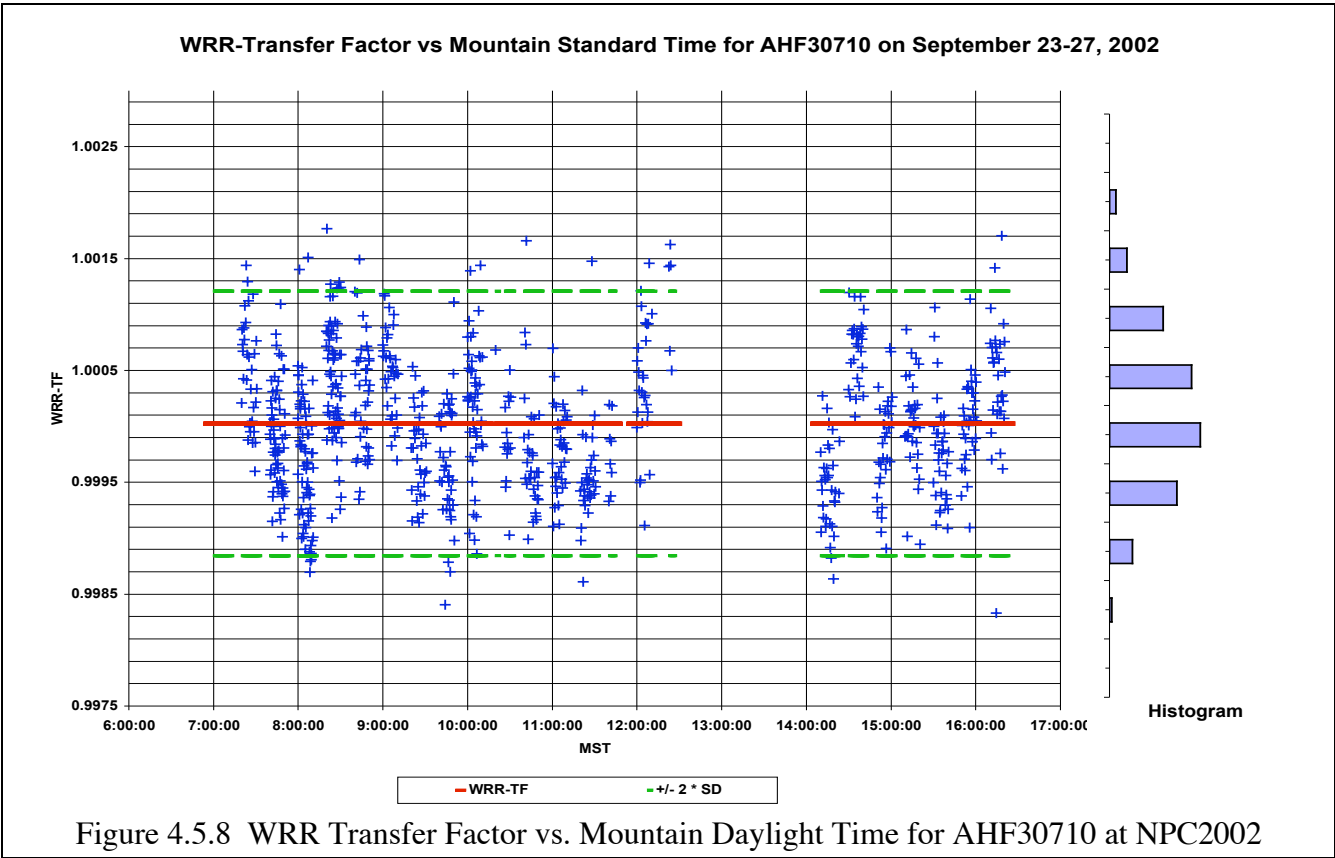

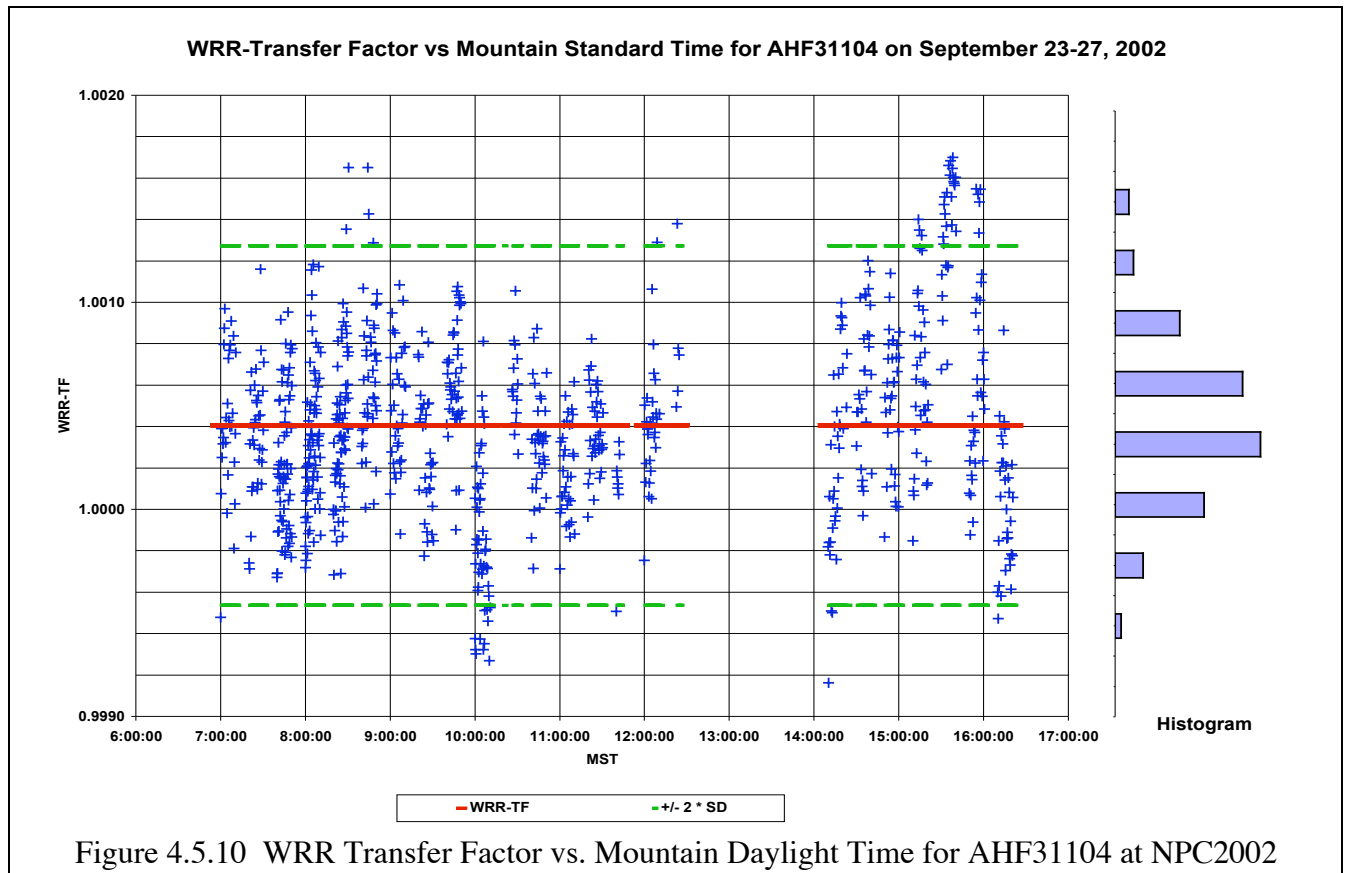


Figure 4.5.10 WRR Transfer Factor vs. Mountain Daylight Time for AHF31104 at NPC2002

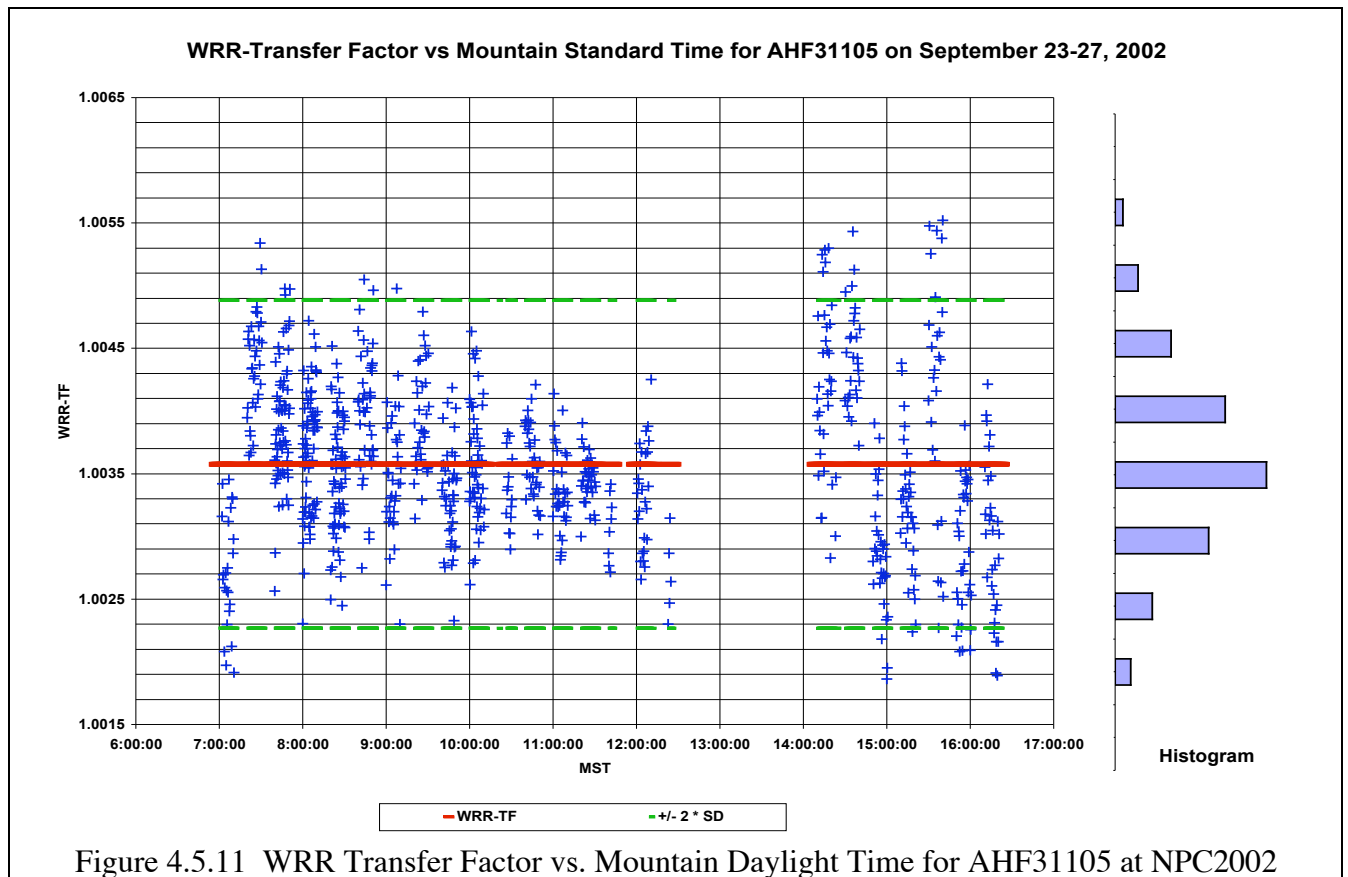
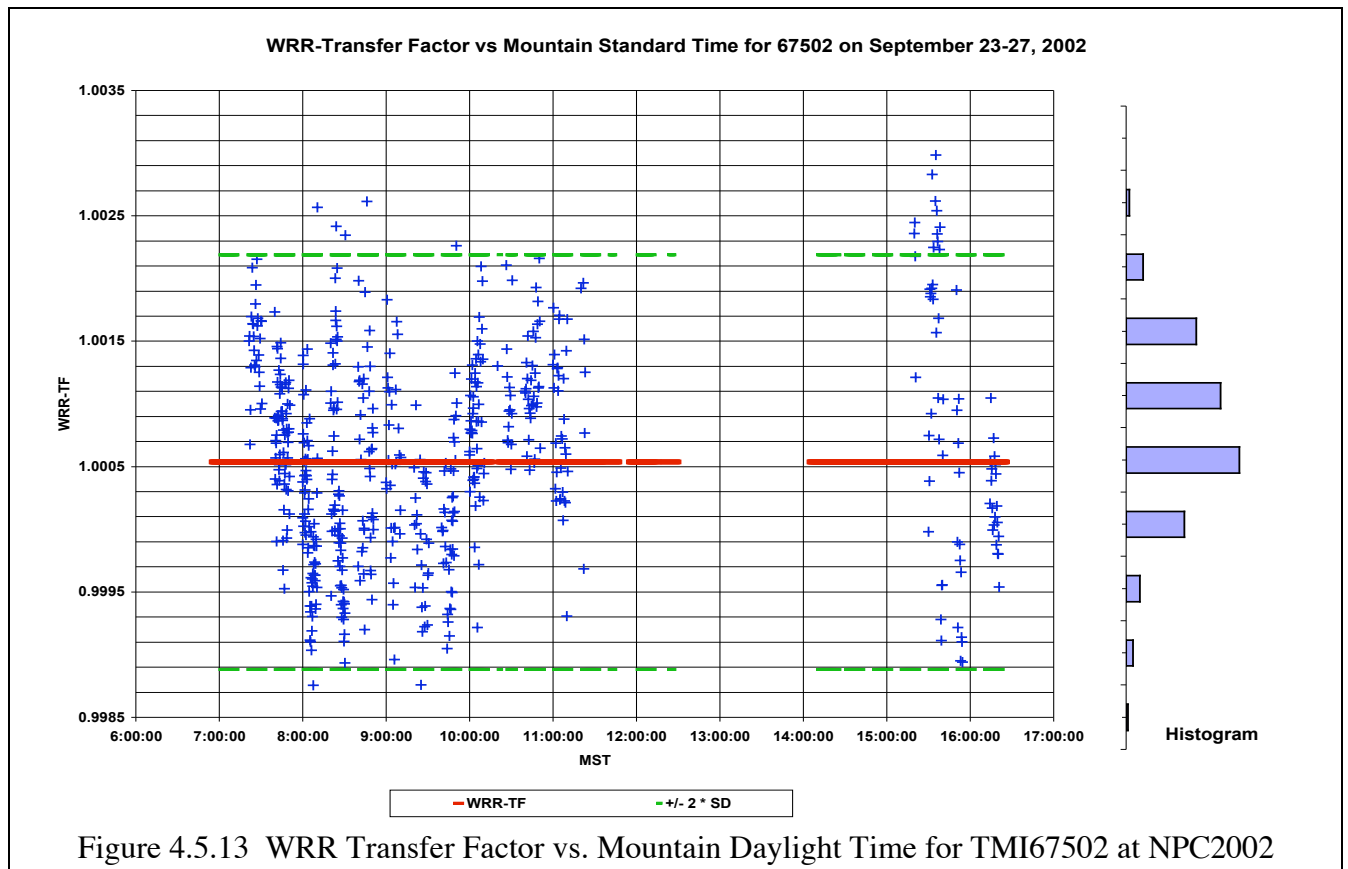
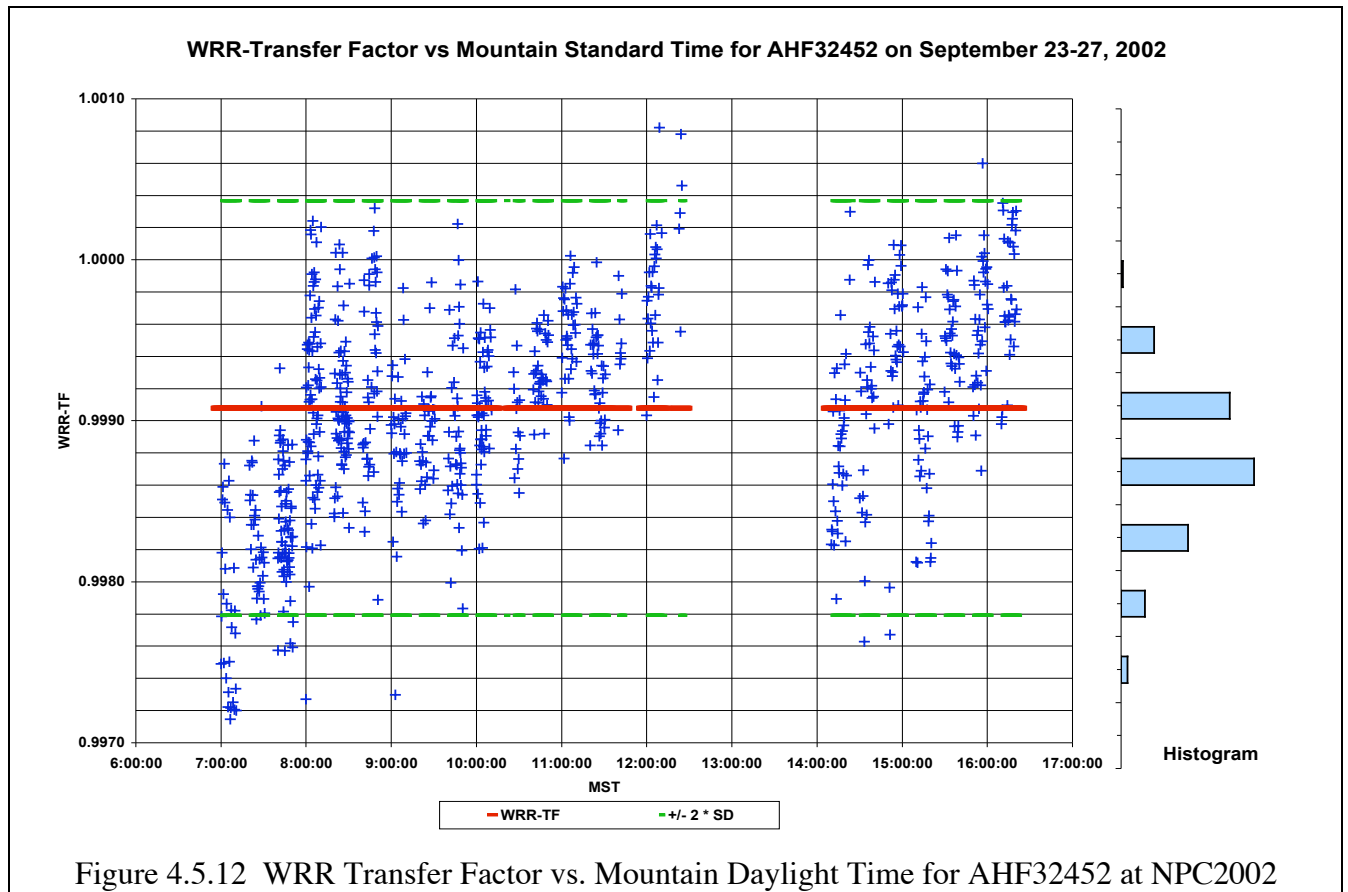


Figure 4.5.11 WRR Transfer Factor vs. Mountain Daylight Time for AHF31105 at NPC2002



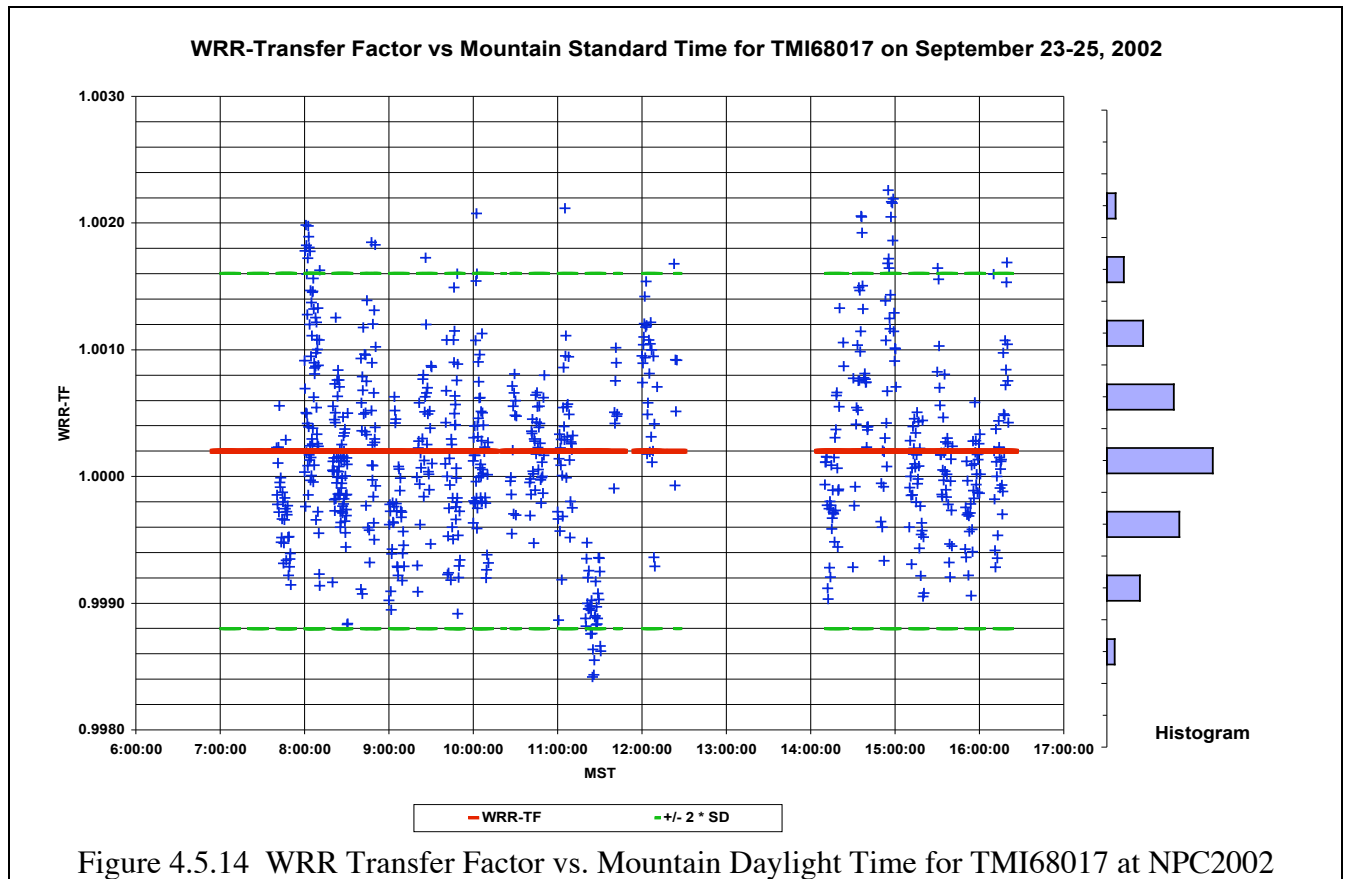


Figure 4.5.14 WRR Transfer Factor vs. Mountain Daylight Time for TMI68017 at NPC2002

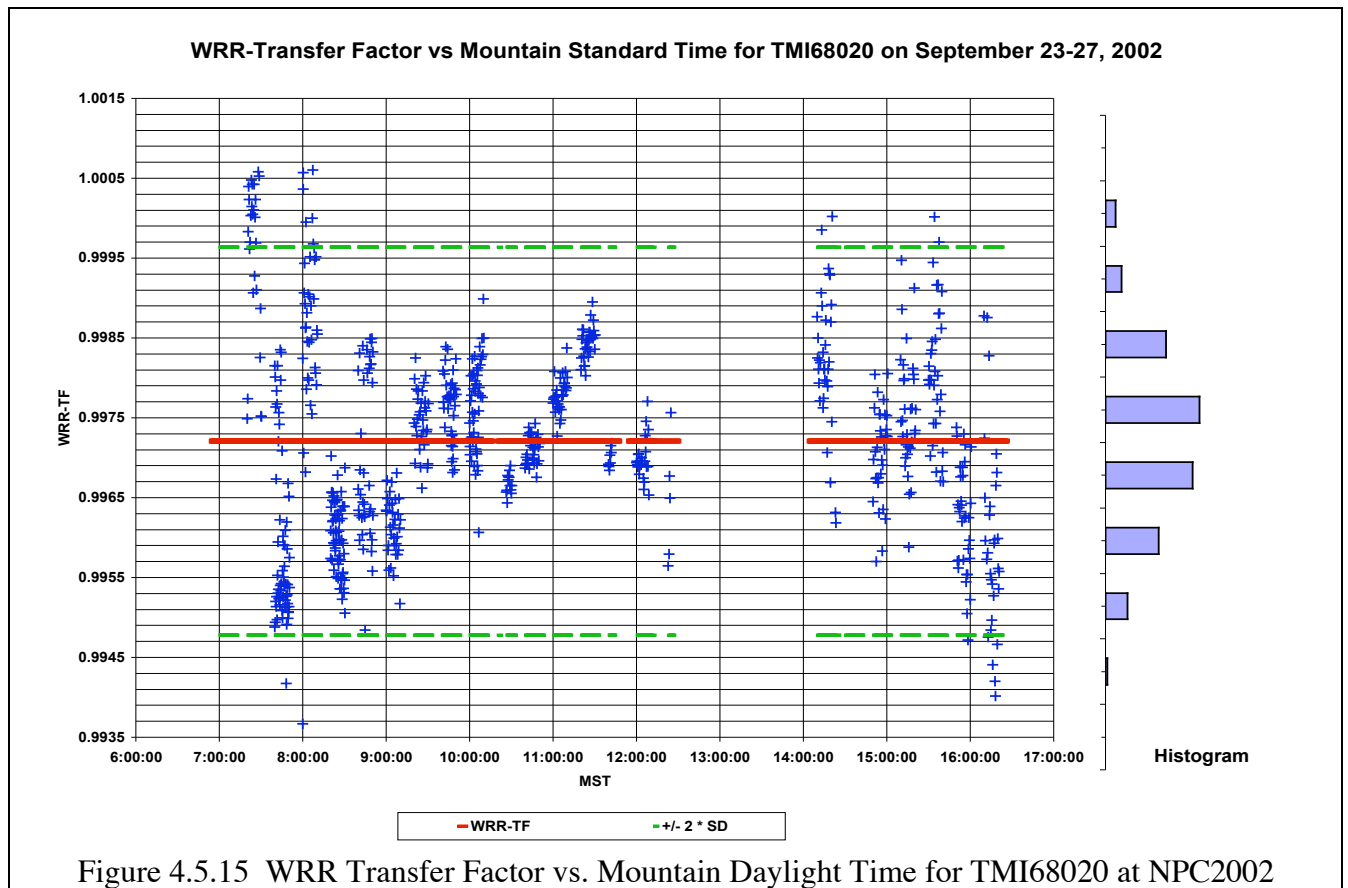


Figure 4.5.15 WRR Transfer Factor vs. Mountain Daylight Time for TMI68020 at NPC2002

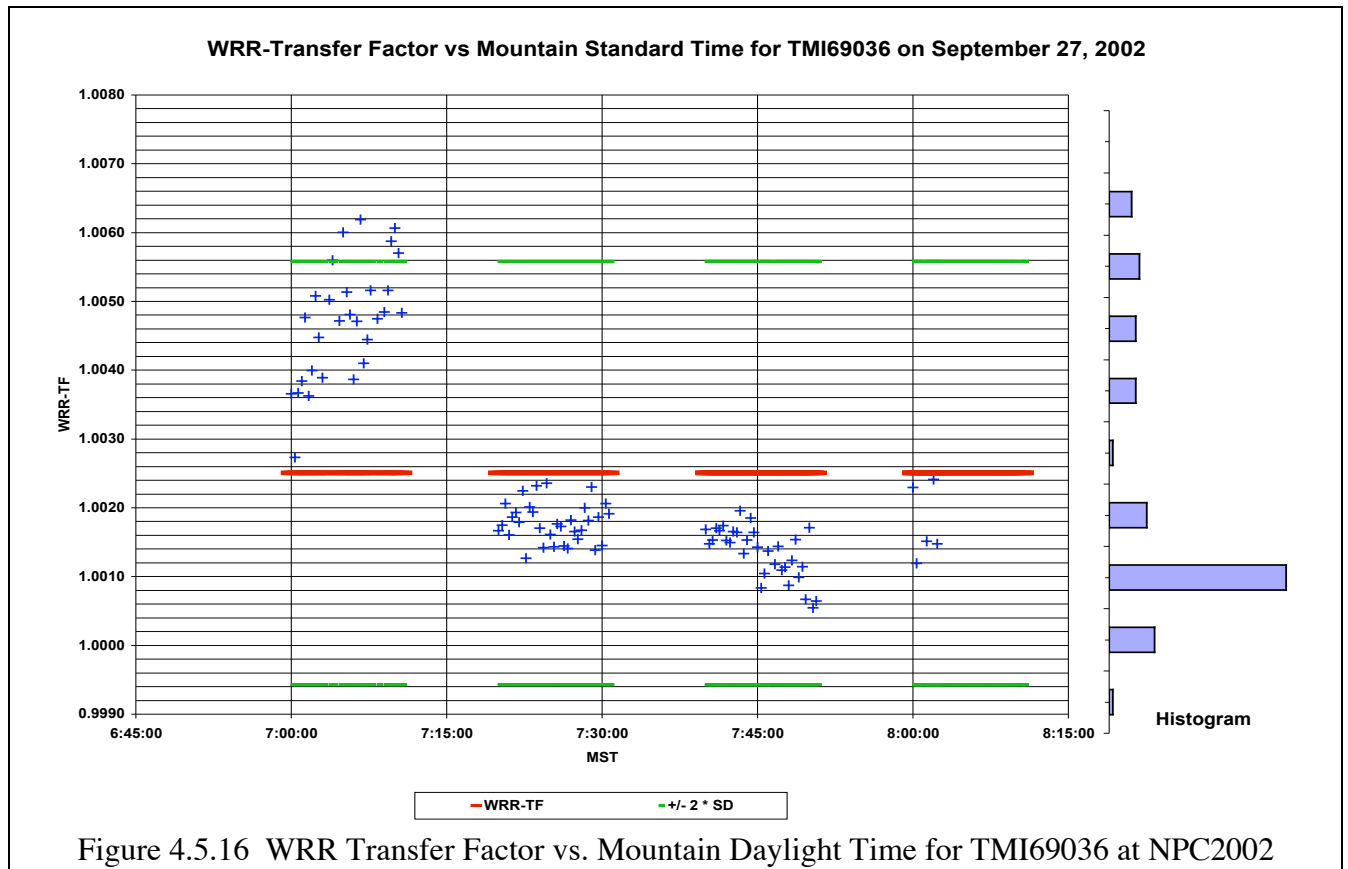


Figure 4.5.16 WRR Transfer Factor vs. Mountain Daylight Time for TMI69036 at NPC2002


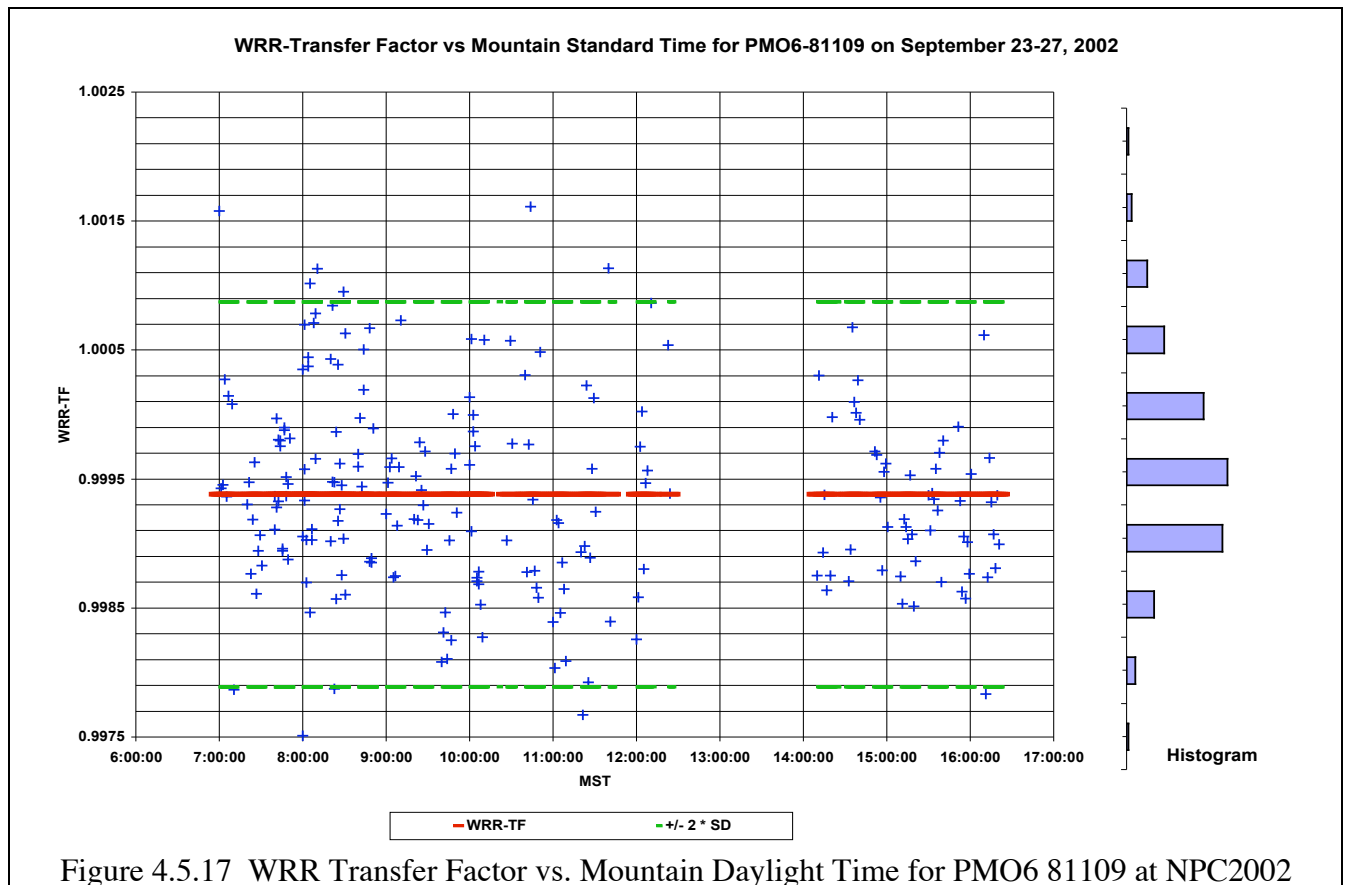


Figure 4.5.17 WRR Transfer Factor vs. Mountain Daylight Time for PMO6 81109 at NPC2002

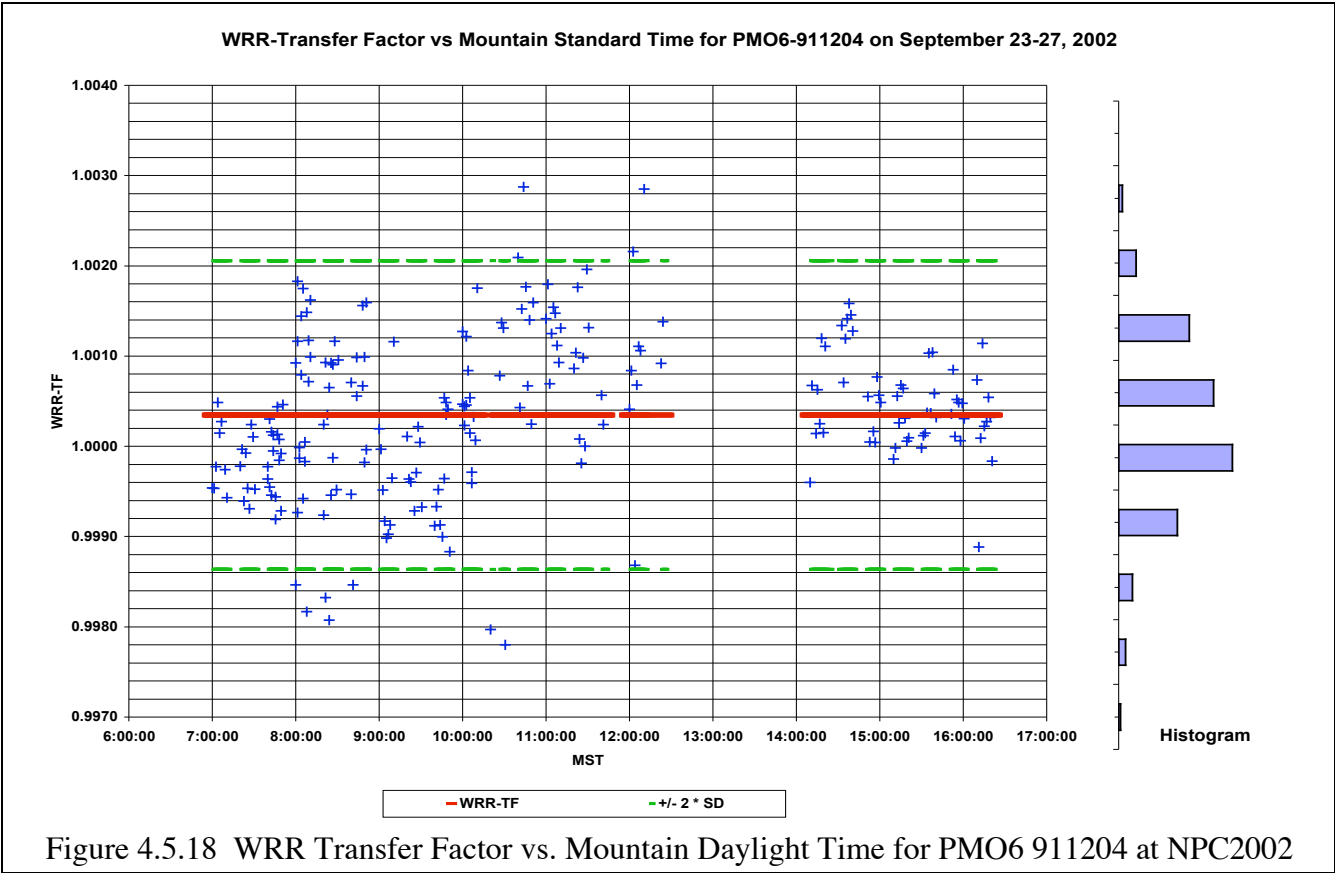

## 4.6 Recommendations

As a result of these comparisons, we suggest the participants observe the following measurement practices:

- For the purpose of pyrheliometer comparisons, such as NPC2002, we recommend the user apply only the manufacturer's calibration factor (CF), not the WRR Transfer Factor or the new calibration factor, to report his/her absolute cavity radiometer's irradiance readings. This eliminates the possibility of compounding WRR factors from previous comparisons.
- For data collection purposes, the manufacturer's CF is used to calculate the cavity responsivity. Each irradiance reading is then *multiplied* by the appropriate WRR Transfer Factor.

For future comparisons, we strongly urge the participants to provide their irradiance readings in the following format:

Serial Number  
##, HH:MM:SS, TPs, IRR

where,

Serial Number	=	Instrument serial number (first line only)
##	=	Reading number (1 to 33) within the Run
HH:MM:SS	=	Hour, minute and second of the reading (Local Standard Time, 24-hour clock)
TPs	=	Measured thermopile signal (mV) with resolution of X.XXXXX
IRR	=	Computed irradiance (Wm <sup>-2</sup> ) with resolution of XXXX.X

The file naming convention is suggested to include the radiometer serial number and date of observations (e.g., *AHF307131009.99* would correspond to data from AHF30713 on 10/9/99).

## 5. **Ancillary Data**

The meteorological elements of temperature, relative humidity and barometric pressure were measured during the comparisons using the meteorological station at SRRL. A NIP, PSP, and Model 8-48 measured direct, global, and diffuse irradiances respectively. These radiometers are used in SRRL's Baseline Measurement System (BMS). The BMS provides 1-minute averages of 3-second samples. Additional information, including data and graphical summaries, can be found at the Measurements and Instrumentation Data Center:

**[http://www.nrel.gov/midc/srri\\_bms](http://www.nrel.gov/midc/srri_bms).**

Time-series plots and other graphical presentations of these data are presented in Appendix B.

## 6. References

- Fröhlich, C., 1991. History of Solar Radiometry and the World Radiometric Reference. *Metrologia*, Vol. 28, Issue 3.
- Reda, I., 1996. Calibration of a Solar Absolute Cavity Radiometer with Traceability to the World Radiometric Reference. NREL/TP-463-20619. The National Renewable Energy Laboratory, Golden, Colorado.
- Romero, J., 1995. Direct Solar Irradiance Measurements with Pyrheliometers: Instruments and Calibrations. IPC-VIII, Davos, Switzerland; 16p.
- Romero, J; N.P. Fox and C. Fröhlich, 1996. Improved Comparison of the World Radiometric Reference and the SI Radiometric Scale. *Metrologia*, Vol. 32, Issue 6 (May), p523-524.
- WRC/PMOD, 1996. International Pyrheliometer Comparison, IPC VIII, 25 September - 13 October 1995, Results and Symposium. Working Report No. 188, Swiss Meteorological Institute, Dorfstrasse 33, CH-7260 Davos Dorf, Switzerland. 115 pp.

## 7. Images

Digital images taken during NPC-2002 are available from the SRRL web site:  
<http://www.nrel.gov/srrl/npc2002>



## Appendix A: List of Participants and Pyrheliometers

<u>Name / Address / Phone / Fax / E-mail</u>	<u>Pyrheliometer(s)</u>
<b>Fred Denn</b> Analytical Services & Materials, Inc. Atmospheric Sciences Group 1 Enterprise Parkway, Suite 300 Hampton, VA 23666-5845 Phone: 757-827-8659 E-mail: F.M.Denn@Larc.NASA.GOV	AHF 31041 AHF 31105
<b>Robert Dolce</b> (sent radiometer) Kipp & Zonen 125 Wilbur Place Bohemia, NY 11716 Phone: 631-589-2065 ext 24 Fax: 631-589-2068 E-mail: robert.dolce@kippzonen.com	CH1 010258
<b>Jim Goza</b> Lockheed Martin Technical Operations P.O.Box 179 MS: P9682 Littleton, CO 80201 Phone: E-mail:	TMI 68020
<b>Bob Heiskell</b> DSET Laboratories 45601 North 47 <sup>th</sup> Ave. Phoenix, AZ 85087 Phone: 623-465-7356 Fax: 623-465-9409 E-mail: bheiskell@atlaswsg.com	AHF 17142

**Gary Hodges**  
NOAA/OAR/ARL/SRRB  
325 Broadway  
Boulder, CO 80305  
Phone: 303-497-6460  
Fax: 303-497-6546  
E-mail: [gary.hodges@noaa.gov](mailto:gary.hodges@noaa.gov)

AHF 30710

**Duncan Maciver**  
DSET Laboratories  
45601 North 47th Ave.  
Phoenix, AZ 85027  
Phone: 623-465-7356  
Fax: 623-465-9409  
E-mail: [dmaciver@atlaswsg.com](mailto:dmaciver@atlaswsg.com)

AHF 17142

**Joe Michalsky**  
Atmospheric Sciences Research Center  
State University of New York at Albany  
251 Fuller Road  
Albany, NY  
Phone: 518-437-8755  
Fax: 518-437-8758  
E-Mail: [joe@asrc.cestm.albany.edu](mailto:joe@asrc.cestm.albany.edu)

HF 28552

**Bill Miller**  
Lockheed Martin Technical Operations  
P.O.Box 179  
MS: P9682  
Littleton, CO 80201  
Phone: 303-977-5996  
Fax: 303-971-5635  
E-mail: [William.b.miller@lmco.com](mailto:William.b.miller@lmco.com)

TMI 68020

**Daryl Myers** (sent radiometer)  
National Renewable Energy Laboratory  
1617 Cole Blvd.  
Golden, CO 80401-3393  
Phone: 303-384-6768  
Fax: 303-384-6391  
E-mail: [myersd@tcplink.nrel.gov](mailto:myersd@tcplink.nrel.gov)

AHF 23734

**Don Nelson**  
NOAA/CMDL  
Climate Monitoring & Diagnostics Laboratory  
M/5 R/CMDL1  
325 Broadway  
Boulder, CO 80305  
Phone: 303-497-6662  
Fax: 303-497-6290  
E-mail: donald.w.nelson@noaa.gov

AHF 28553  
TMI 67502  
AWX 32448

**Ibrahim Reda**  
National Renewable Energy Laboratory  
1617 Cole Blvd.  
Golden, CO 80401-3393  
Phone: 303-384-6385  
Fax: 303-384-6391  
E-mail: Ibrahim\_Reda@nrel.gov

AHF 23734  
AHF 28968  
AHF 29220  
AHF 30713  
AHF 31104  
AWX 32452

**Tom Stoffel**  
National Renewable Energy Laboratory  
1617 Cole Blvd.  
Golden, CO 80401-3393  
Phone: 303-384-6395  
Fax: 303-384-6391  
E-mail: Tom\_Stoffel@nrel.gov

TMI 68017  
TMI 68018  
TMI 69036

**Jim Treadwell**  
NOAA/CMDL  
Climate Monitoring & Diagnostics Laboratory  
M/5 R/CMDL1  
325 Broadway  
Boulder, CO 80305  
Phone: 303-497-6654  
Fax: 303-497-6290  
E-mail: James.Treadwell@noaa.gov

AHF 28553  
TMI 67502  
AWX 32448

**Craig Webb**  
Atmospheric Radiation Measurement Program  
ARM Program Site Office  
309600 EW 28  
Billings, OK 74630-2045  
Phone: 580-388-4053  
Fax: 580-388-4052  
Email: craigw@ops.sgp.arm.gov

AHF 28964  
AHF 29222  
AHF 30495

**Wim Zaaiman**  
European Commission Directorate General JRC  
Environment Institute  
Renewable Energies Unit  
Building 45, TP450  
Via Fermi, 1  
I-21020 Ispra (Va), Italy  
Phone: + 39 0 332 785 750  
Fax: +39 0 332 789 628  
E-mail: willem.zaaiman@jrc.it

PM06 81109  
PM06 911204  
CH1 010258 <control  
CH1 930018 <control

#### **NREL Staff**

<b>Afshin Andreas</b>	Computer Issues (Virus scan, E-mail, Web Site)
<b>Pete Gotseff</b>	Tools, Parts (Electronics and Hardware), Trackers
<b>Bev Kay</b>	Facilities and services (Phone, Mail, Food)
<b>Ibrahim Reda</b>	NPC Data Collection & Processing, Cavity Operations
<b>Tom Stoffel</b>	Host (Security, Safety, Logistics, Food)
<b>Steve Wilcox</b>	Computer Issues, Trackers, Cavity Operations

**Appendix A (concluded):  
List of Pyrheliometers**

<u>No.</u>	<u>Serial No.</u>	<u>Owner / Application</u>
1	AHF 17142	Atlas Weathering Services-DSET Labs / Reference Standard
2	AHF 23734	NREL / Photovoltaics Program Reference
3	HF 28552	State University of New York at Albany, Atmospheric Sciences Research Center / Reference
4	AHF 28553	NOAA Climate Monitoring & Diagnostics Laboratory (CMDL) / Reference
5	AHF 28964	U.S. Department of Energy (DOE) Atmospheric Radiation Measurement (ARM) Program / Southern Great Plains Site Reference
6	AHF 28968	DOE ARM/ Program Reference
7	AHF 29220	NREL / Metrology Lab Reference Standard #2
8	AHF 29222	DOE ARM-Southern Great Plains / All-Weather
9	AHF 30495	DOE ARM-Southern Great Plains Working Standard
10	AHF 30710	NOAA / Surface Radiation Research Branch Reference
11	AHF 30713	NREL / Metrology Lab Working Standard #1
12	AHF 31041	NASA Clouds and the Earth's Radiant Energy System (CERES) / Reference 1
13	AHF 31104	NREL / Metrology Lab Working Standard #2
14	AHF 31105	NASA Clouds and the Earth's Radiant Energy System (CERES) / Reference 2
15	AWX 32448	NOAA / CMDL All-Weather Standard
16	AWX 32452	NREL / All-Weather Standard
17	PMO6 81109	European Commission Directorate General / Reference Standard
18	PMO6 911204	European Commission Directorate General / Reference Standard
19	TMI 67502	NOAA CMDL / Reference Standard
20	TMI 68017	NREL / SRRL All-Weather BORCAL Working Standard #2
21	TMI 68018	NREL / Metrology Lab Reference Standard #1
22	TMI 68020	Lockheed-Martin Technical Services / Reference Standard
23	TMI 69036	NREL Metrology Lab / BORCAL Working Standard #3

**Other Pyrheliometers**


1	CH1 930018	European Commission Directorate General / Control Standard
2	CH1 010258	Kipp & Zonen Pyranometer w/ CaF2 Window

## **Appendix B: Ancillary Data Summaries**


The measurement performance of an absolute cavity can be affected by several environmental parameters. Potentially relevant meteorological data collected during the NPC are presented in this appendix. The Baseline Measurement System (BMS) has been in continuous operation at the Solar Radiation Research Lab (SRRL) since 1985. BMS data are recorded as 1-minute averages of 3-second samples for each instrument. Additional information about SRRL and the BMS can be found at our Measurement & Instrumentation Data Center: [http://www.nrel.gov/midc/srrl\\_bms](http://www.nrel.gov/midc/srrl_bms).

Time-series plots and other graphical presentations of these data acquired during the NPC-2002 measurements are presented here.


# Baseline Measurement System Data for September 23, 2002

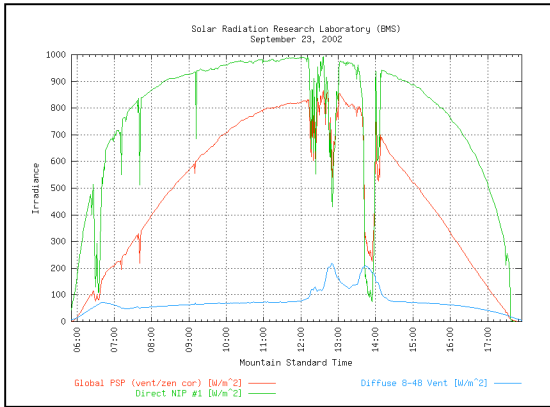


Broadband Irradiance

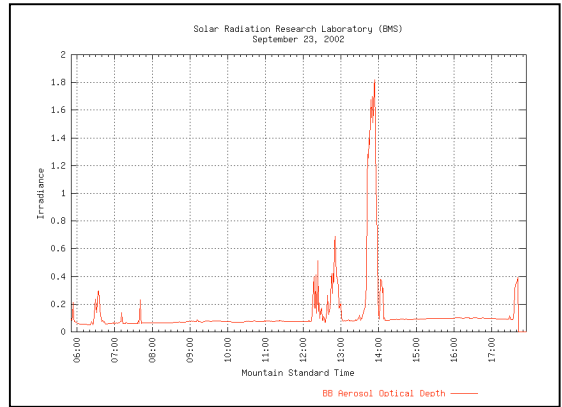


Aerosol Optical Depth

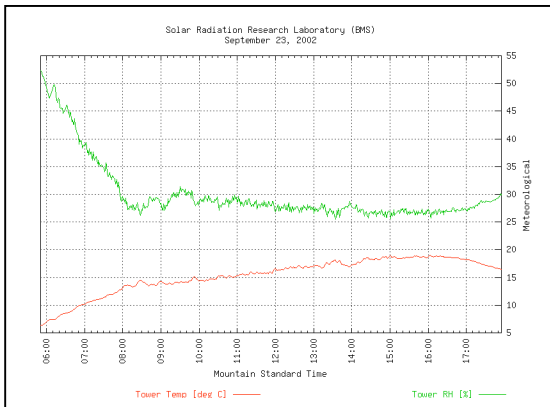


Temperature & Relative Humidity

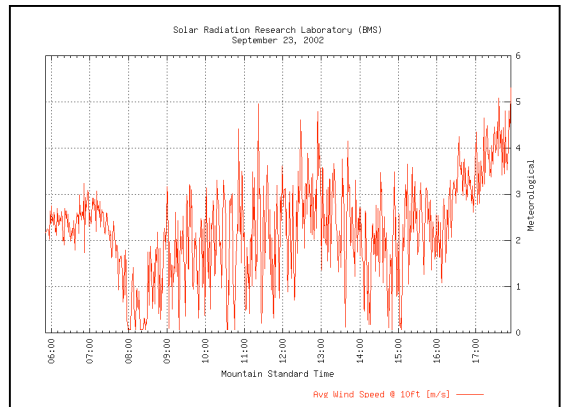

Wind Speed at 10 m AGL

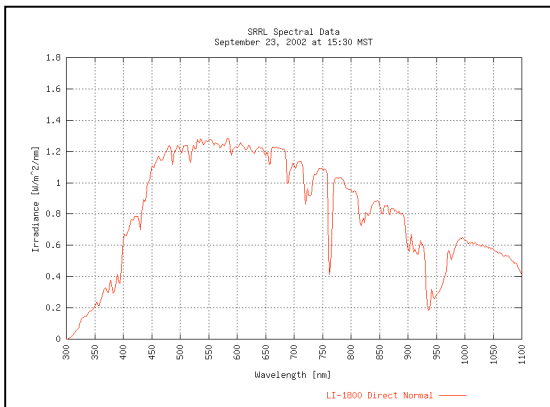


Direct Normal Spectra

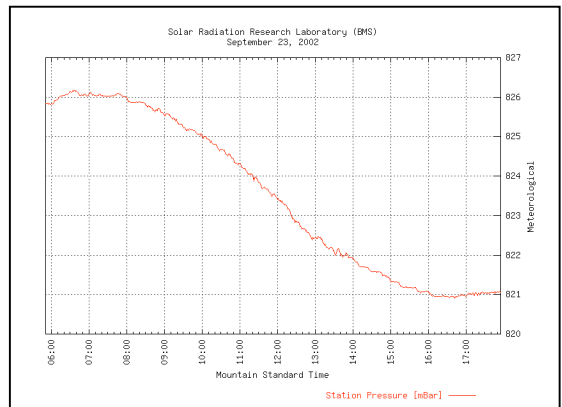


Station Pressure


# Baseline Measurement System Data for September 24, 2002

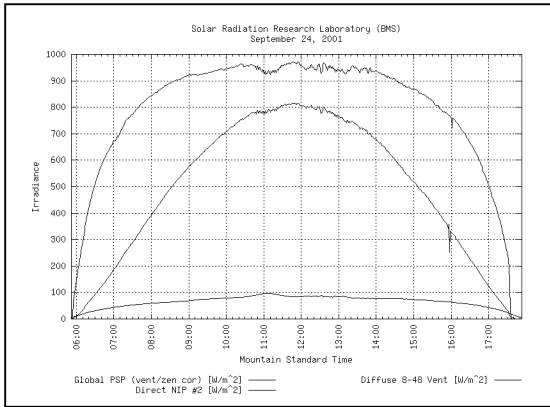


**Broadband Irradiance**

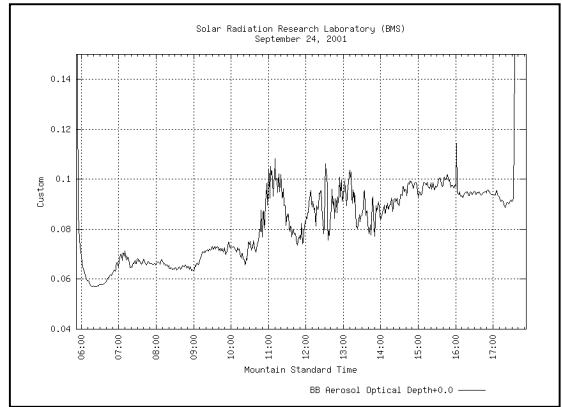


**Aerosol Optical Depth**

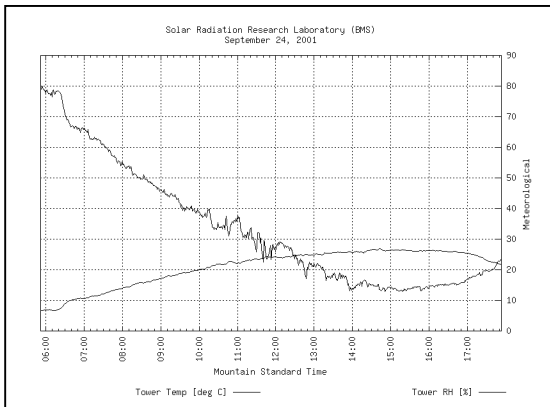


**Temperature & Relative Humidity**

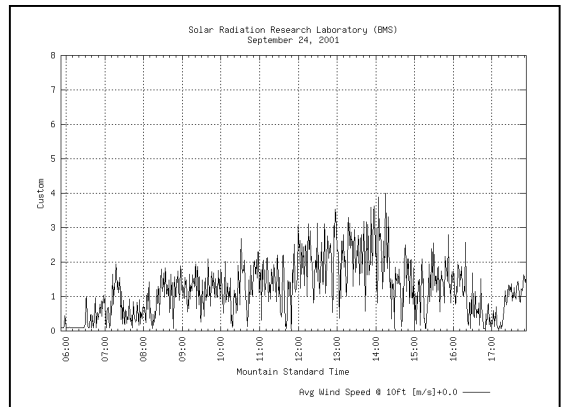

**Wind Speed at 10 m AGL**

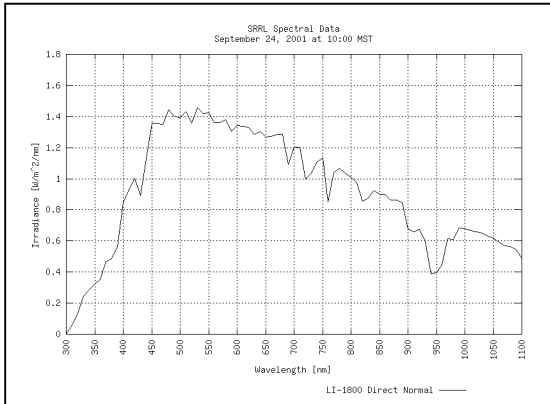


**Direct Normal Spectra**

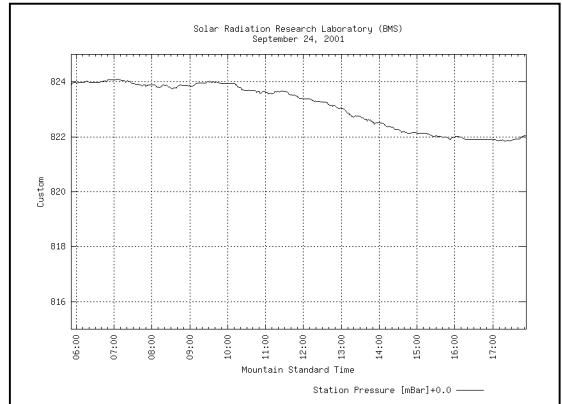


**Station Pressure**




# Baseline Measurement System Data for September 25, 2002

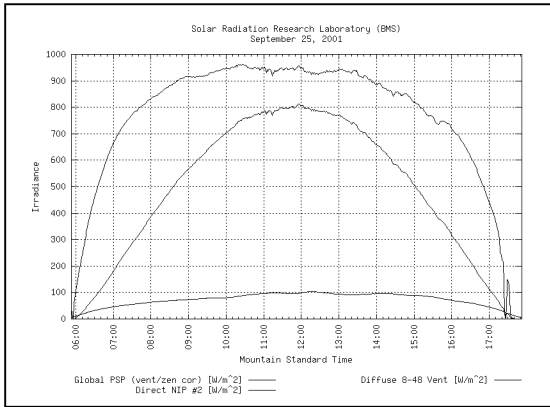


**Broadband Irradiance**

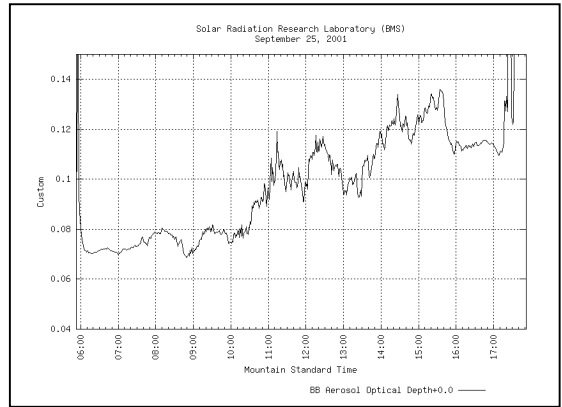


**Aerosol Optical Depth**

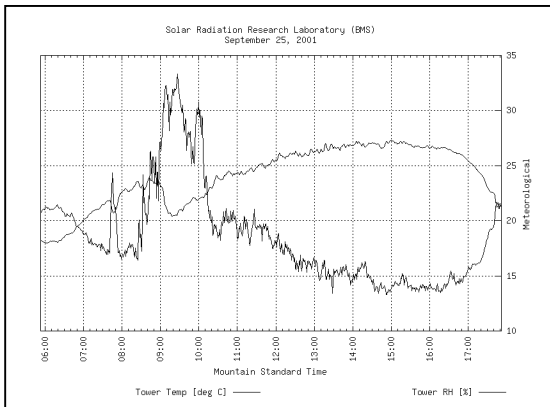


**Temperature & Relative Humidity**

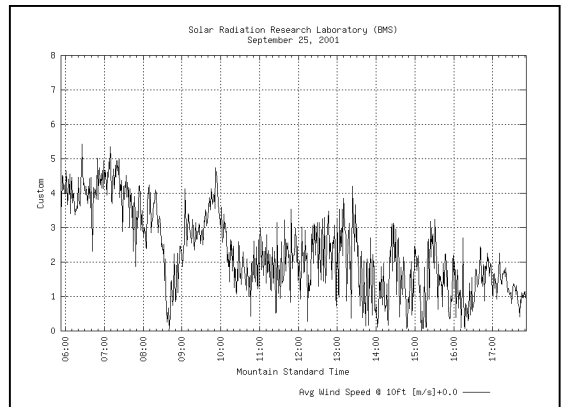

**Wind Speed at 10 m AGL**

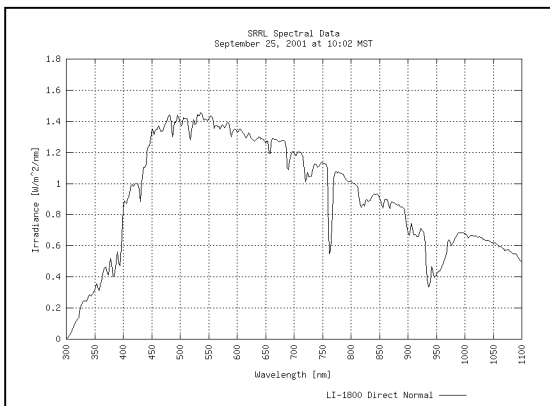


**Direct Normal Spectra**

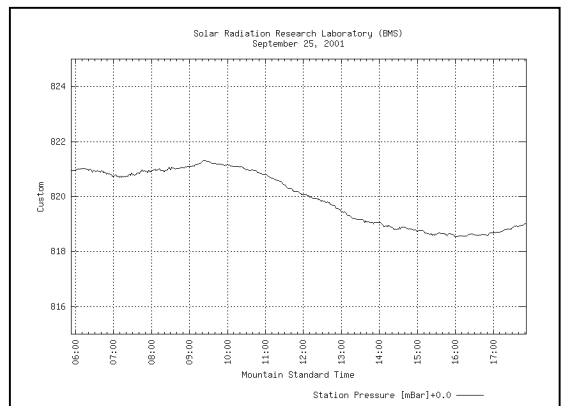


**Station Pressure**


# Baseline Measurement System Data for September 26, 2002

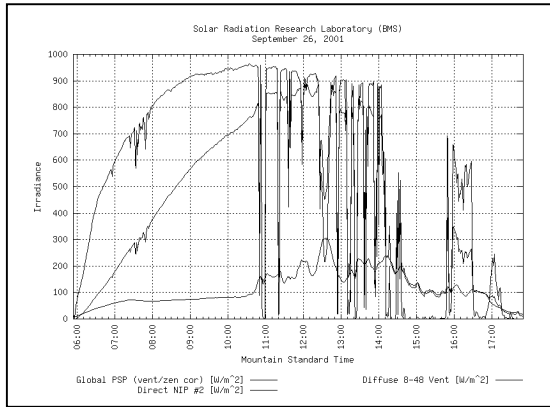


Broadband Irradiance

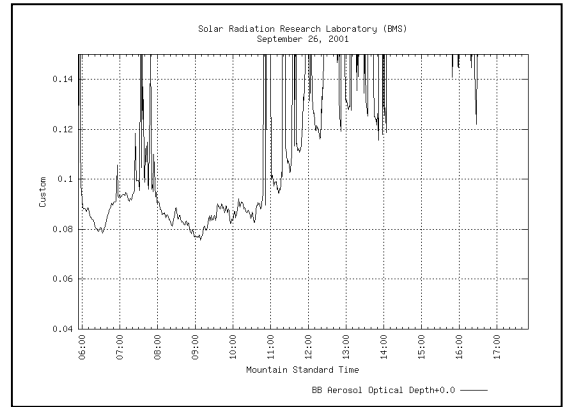


Aerosol Optical Depth

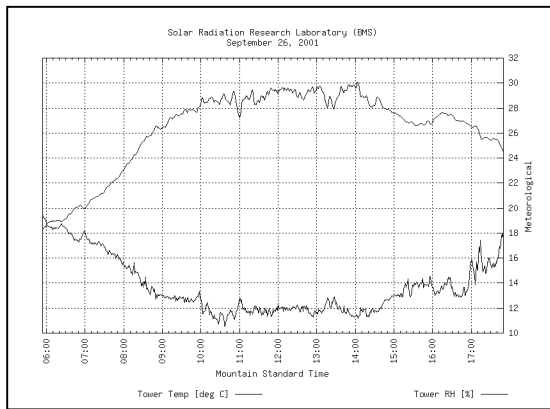


Temperature & Relative Humidity

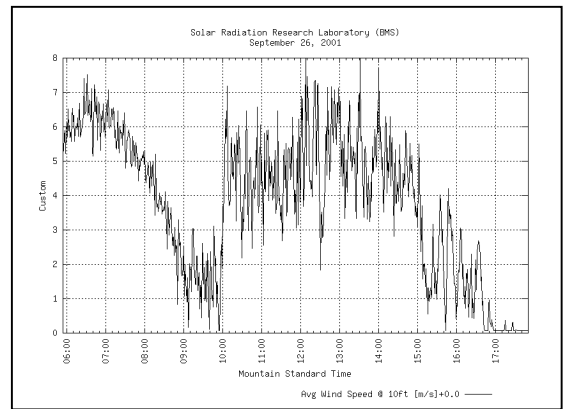

Wind Speed at 10 m AGL

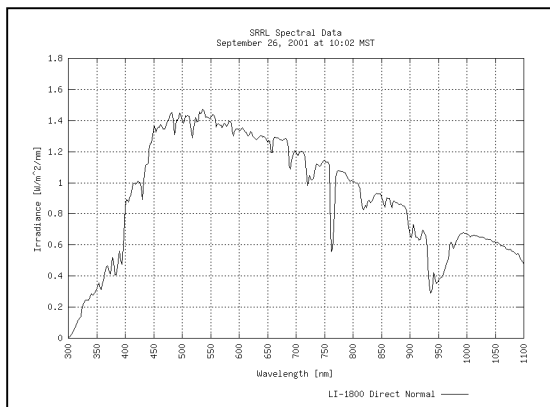

Direct Normal Spectra

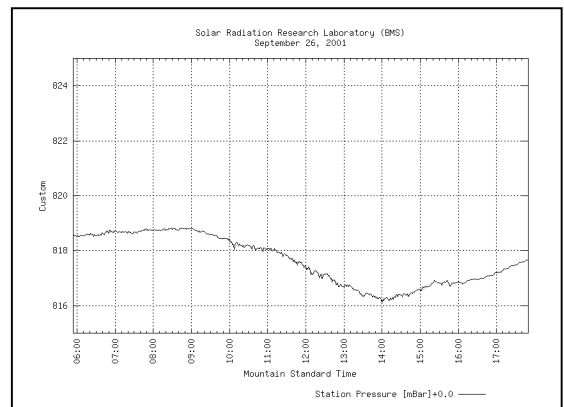

Station Pressure

## Appendix C: Operational Notes

The following text was distributed to the participants at the opening of the NPC for discussion to achieve consensus.

### 2002 Absolute Cavity Radiometer Comparisons at NREL Protocol Issues Summary

Based on past experiences, we need to agree on the following issues before we begin the comparisons.

1. Title - We will refer to this effort as *NPC-2002* (NREL Pyrheliometer Comparisons 2002).

2. Schedule -

Please call Tom's voice mail (303-384-6395) after 06:30 MDT for recorded announcement of daily plan:

**Clear** sky forecast = Data!                      **Cloudy** = Conference Room FTLB 153.

September 23<sup>rd</sup> :

07:30 - 08:30-Visitor check-in at Site Entrance Building.

08:00 - 12:00-Transport equipment to SRRL.

-Equipment Installation & tests.

-ALL personal computers will be scanned for viruses prior to their use at SRRL.NREL will provide this service. A seating diagram is available to indicate operator/solar tracker assignments, but we'll see how this works once every one's there.

12:00 - 13:00-Lunch

13:00 - 17:00-Continue equipment tests as needed

-Review measurement protocol, data format and procedures.

-Dry-run(s) of comparison measurements (weather permitting)

-Update Attendance List Information.

September 23<sup>rd</sup> - October 4<sup>th</sup> (including weekends):

• **Clear sky** => Measurements!

08:00                      -Arrive at SRRL

08:00 - 08:30-Deploy instruments

08:30 - 09:00-Equipment warm-up for at least 30-minutes

09:00 - 17:30-Comparison Data Collection

-Measurements until sundown or clouds.

September 23<sup>rd</sup> - October 4<sup>th</sup> (including weekends):

- **Cloudy sky** => No Measurements, but optionally...

Conference Room 153 in Building "FTLB" is reserved daily for our use:

- Review of previous day's data analyses
- Technical Briefings on Radiometry
- Equipment Tests
- NREL Tours
- Office Time (limited e-mail connections at SRRL)

We will determine the need for more measurements at the end of each day.  
(see item 5 below)

### 3. SRRL Coordinates

Program your solar tracker using:

LAT = 39.7425 N  
LON = 105.1778 W  
ELEV = 1828.8 m AMSL (6,000 ft)  
BARO = 820 mBar (average station pressure)

### 4. Time Keeping

- A timekeeper will be identified.
- All time records will be Mountain Standard Time (MST)
- The NIST atomic clock is a local call:  
303-499-7111
- A GPS time source is also available.
- Set your system clock at the daily start-up or as often as needed for 2 sec accuracy.

### 5. Minimum Data Set

A subject for discussion, but 300 data points (your instrument/Reference) could be our goal for a minimum data set for these comparisons.

### 6. Measurements

- Do NOT apply any previous WRR correction factors to your measurements.
- Use only the factory calibration factor to adjust your data beyond any other adjustments you feel are needed to correct your data (e.g., pre- and post-calibration drifts in sensitivity are OK).As in the past, we will use the following terms:

<i>Calibrate</i>	=	Perform electrical calibration and wait for next measurement period to begin
<i>Reading</i>	=	A measurement of direct irradiance within 1 sec of announcement at 20-sec intervals.
<i>Run</i>	=	Collection of 31 readings taken in sequence.
<i>Shade &amp; Calibrate</i>	=	Perform electrical calibration after each run.

The timekeeper will make the following announcements for each Run:

- Next Run Begins at HH:MM (MST)
- T minus 6 minutes. Begin calibration
- T minus 3 minutes
- T minus 2 minutes
- T minus 1 minute
- T minus 30 sec
- T minus 10 sec
- T minus 5 - 4 - 3 - 2 - 1 - READ!
- READ! (at T plus 20 sec intervals for 33 readings in a *Run*)

7. Data Transfer

The data format will be discussed on the first day. After the last daily RUN, but before equipment teardown, our Data Keeper (TBD) will circulate a master diskette for you to copy all of your corrected data. Calibration files will not be collected.

8. Data Processing

Reda has developed an Excel spreadsheet system for reducing the data.

9. Data Reporting

Our goal is to provide each participant with next-day analyses. A final report will be published by NREL within two months of the comparisons.

10. Equipment Storage

Each participant will be given space to store systems at SRRL. Please let us know if you wish to have any electronics connected to AC power while in storage.

11. Common Sense & Courtesy

Please get permission of owner/operator before touching someone else's equipment!  
(Turn on/off power strips, move cables, etc.)

12. Clean-up

NPC2002 will conclude after all items are returned to the proper storage locations.

13. Contacts

Daily Voice Mail Announcement: **NREL EMERGENCY Press 1234**  
Tom Stoffel .....(303) 384-6395

Questions after normal business hours:  
Tom Stoffel .....(303) 666-9719

Other friendly NREL staff:  
Reda .....(303) 384-6385 <Metrology Lab>  
Pete Gotseff .....(303) 384-6327 <Electronics Lab>  
Bev Kay.....(303) 384-6388 <Solar Radiation Research Lab>  
  
SRRL.....(303) 384-6326 <Let it RING!>